



Analog Transmitter device

MAT 4191 with software extension

- Analog evaluation signal
- Display of % / mA / Pulses
- Analog output 4 – 20 mA
- Limit value with Relayoutput
- for Impedance Measurement
- Drift memory
- Dynamic limit value

- MAT-Version V1.1x
- Technical specifications
- Operating
- Commissioning
- Installation

mipromex
for monitoring product
measurements values



Sales: **Aquasant Messtechnik AG**
Hauptstrasse 22
CH - 4416 Bubendorf / Switzerland
T. +41 (0)61 935 5000

info@aquasant-mt.com
www.aquasant.com

Manufacturer: **Aquasant Messtechnik AG**

Manual No.: VEB-Mipromex-MAT4191-V1.1x_ATEX22

Version: V22103/4

Pages: 46

Author: R. Inauen

Modifications: Subject to modifications

© 2022 Aquasant Messtechnik AG claims copyright protection for this document. The document may not be modified or supplemented without prior written consent. We reserve the right to make changes to technical details compared to the description, information and illustrations in these operating instructions.

change index

Version	Date	Description
2.00	01.2022	Second edition, new Ex certification

Using this manual

Symbols and conventions

- In this document the following conventions are used at formatting to differentiate text elements.
- The names of equipment pieces are written in BOLD.
Example: **mipromex**

In this document the following terms and symbols are used for special program messages:

Emphasized symbols and notices and their meaning:



















	Mortal Danger: the non-observance can lead to injuries or death.		Step by step: Text enhanced/marked this way, contains detailed instructions and comments
	Caution: the non-observance can lead to equipment damages or loss of information.		Actions to be carried out by user.
	Information / Notice: describes equipment characteristic features.		Read and follow instruction steps.
	A waiting time is required during which the equipment does recalibrate itself.	<i>mipromex display</i>	Compare with the mipromex display.
	Adjustment of the measuring electronic MTI (visualized by red and green LED's).		Plug in mains 230/115 V (24 V AC/DC).
	Observe and control equipment display.		Send equipment back to manufacturer.
	Button on mipromex front panel		mipromex Error message on display with Time/Date
	Function: change value according to displayed character set		Button on mipromex front panel
	Change line without store		Function: select number or character
	Button on mipromex front panel, Function: back	ok	Button on mipromex front panel, Functions: menu, select, next, store (press more than 2s)
"next step" in navigation bar	press ok button on mipromex . Press less than 2 seconds to advance to the next parameter	"store" in navigation bar	press ok button on mipromex . Press more than 2 s to store

Chart 1 Symbol description

Index

1. Security and precautions	6
1.1. Installation	6
1.2. Setup	6
1.3. Hazardous Area protection	6
1.3.1. Following notices must be observed:	7
1.4. SIL Safety Integrity Level	7
1.5. Cleaning of units	7
1.6. Maintenance	7
1.7. Warranty claims	7
1.8. Waste disposal of electrical and mechanical components	7
2. mipromex type description	8
2.1. MAT-Hardware types	8
2.1.1. mipromex type code:	9
2.2. Software Versions	10
2.2.1. Basic	10
2.3. Basic functions	11
2.4. Measuring circuit	11
2.5. Function	11
2.1. Measured values processing	12
2.1.1. Static measure processing mode	12
2.1.2. Dynamic measure processing mode	12
3. Structure of data input (parameterization)	13
3.1. General	13
3.2. Key functions	13
3.2.1. Input / changing of characters	13
3.2.2. Select language	13
3.3. Graphic display	14
3.3.1. Display at switch-on of mipromex	14
3.3.2. Measured value display	14
3.3.3. Menu parameter settings	15
4. Program structure with parameters of the analog transmitter	16
4.1. Description of the menu, program structure General, for all mipromex units	19
4.1.1. [1.] Basic settings	19
4.1.2. [2.] Device specs	22
4.1.3. [3.] Signal settings	23
4.1.4. [5.] Measuring range	25
4.1.5. [6.] Limit value	25
4.1.6. [7.] Test functions	27
4.1.7. [8.] Programmable mA output	28
4.1.1. [12.] Calculation parameters	28
5. Commissioning example	30
5.1. Commissioning the mipromex with a pipe probe	30
5.1.1. Detection of water in petrochemical products	30

5.1.2. Oil detection in process- or rain-water-----	30
5.2. Commissioning the mipromex with a bar probe -----	31
5.2.1. Oil detection in process- or rain-water with float -----	31
5.2.2. Foam detection -----	31
5.3. Electronic callbration MTI, basic equalization -----	32
5.4. Inspection release of the parameters -----	33
6. Fault finding -----	35
6.1. After power on -----	35
6.2. During operation-----	35
6.2.1. Data error -----	35
6.2.2. Display error -----	37
6.2.3. Radio equipment -----	37
7. Wiring diagram -----	38
7.1. Measuring electronic/probe with fix connection -----	38
7.2. Connections to female multipoint connector with 32 poles, type: MAT 419* -----	39
7.3. Printed circuit board for 19"-Rack, Monorack, Wall- and Table Top housing-----	40
7.4. Earthing of microprocessor units and probes -----	41
8. Technical Data -----	42
8.1. mipromex Analog transmitter type: MAT 419x -----	42

1. Security and precautions

The following points must be considered at installation and setting up of microprocessor units 24 V AC/DC:

1.1. Installation

- ⇒ The units are IP20 according to EN 60529 and must be protected against e.g. splash water or pollution exceeding the degree of pollution 2.
- ⇒ The units must be installed outside the hazardous area.
Maximum 7 units can be installed into a 19"-Rack. Multipoint connector type: F132 must only be equipped with d- and z – contacts. Solder connections are to be isolated with heat shrinkable sleeves (see chapter 7.2)
- ⇒ Single units installed with Monorack Type: MRM 2 (see chapter 7.4)
Housings or switch cabinets must be ventilated (dissipation of heat built-up)
- ⇒ Hazardous area blue line to lead separately (cable channel or joined to loom of cables)
Equipotential bond must be installed; Hazardous area protection
Outside installations: a corresponding lightning protection of the probe supply cables is recommended.
- ⇒ Installation instructions for impedance probes I must be observed

1.2. Setup

- ⇒ Verify wiring and power supply tension (chapter 7.2)
- ⇒ Perform probe and system specific parameterization in the menu (chapter 5)
- ⇒ Check max. load of the opto-electronic coupling transistor outputs (NPN) according to datasheet (chapter 7.6)
- ⇒ Adjustments under tension are only allowed to be carried out by manufacturer
Handling by user is performed only via protected film keypad
Repair of unit only by trained personnel with manufacturer certificate

1.3. Hazardous Area protection

Control devices with intrinsically safe output, approved for the connection of defined rod probes in the Ex zone according to SEV ATEX22.



The EU type examination certificate must be observed. Compliance with the "Special Conditions" contained therein is particularly important. Ex certification according to directive RL 2014/34/EU

Please note the following documents:

- *VDZ-SEV22-ATEX-ISO_Zertifkat-Doc.pdf* (currently valid certificates)
- *VDD-STM*** ...Technical probe data sheet with the specific (X) Ex-relevant layer thicknesses and information about use in which zone.

1.3.1. Following notices must be observed:

1. The microprocessor control unit **mipromex** as per EN 60079-0:2006 can only be used outside of the hazardous area.
2. The highest allowed ambient temperature is 60°C (also inside a protective housing)
3. The microprocessor unit **mipromex** is to install in a manner that at least the protection standard IP 20 as per Standard IEC 529 resp. EN 60529 is fulfilled. By corresponding mount into rack unit this condition is fulfilled.
4. At installation of the microprocessor control unit **mipromex** a minimum distance of 50mm must be created by insertion of a separation wall between the intrinsic safe and non intrinsic safe wiring circuit or the connecting parts must be insulated (i.e. with a heat-shrinkable sleeve). The input lines are secured to the rack or the monorack with a strain relief.
5. The intrinsic safe signal wiring circuits are safe galvanic separated from the remaining wiring circuits up to a peak value of 375 V of the nominal voltage

1.4. SIL Safety Integrity Level

The microprocessor unit **mipromex** is produced as per the SIL standards Norm IEC 61508/61511.

1.5. Cleaning of units

The microprocessor unit **mipromex** and the measuring electronic **MTI** built-in on the probe head are not allowed to be cleaned with water.

The cleaning of the front panel is to be done with a slightly dampened, clean cloth. The printed circuit boards, to remove the dust, shall only be slightly blown-out with compressed air (low pressure 4 bar).

The bar probes must be cleaned with alcohol or a corresponding solvent.

Probes with stainless steel electrodes (SRK or SRM or probes made to measure powders/solids) are not allowed to be cleaned with water or liquids.

1.6. Maintenance

The data transmission of the microprocessor units remains stable, even over a long period of time. Therefore, a periodic adjustment or similar, is not necessary.

1.7. Warranty claims

Your measuring system had to undergo a precise final inspection at the factory. Interventions are only allowed to be carried out by a competent person. Warranty according to Aquasant Messtechnik AG warranty.

1.8. Waste disposal of electrical and mechanical components



The Waste Electrical and Electronic Equipment (WEEE) Directive, which came into force on 13 February 2003, has brought about a major change in the way we handle electrical and electronic equipment that is no longer used. The WEEE logo (see on left), either on the product itself or on the packaging, indicates that this product must not be disposed of with normal household waste. For more information regarding the disposal of waste electrical and electronic equipment and for recycling and collection points, please contact your relevant local authority or the business where you purchased the device.

2. mipromex type description




Pic. 1 mipromex

2.1. MAT-Hardware types

MAT 4190	1 measuring circuit with 1 analog output and 1 limit value output Relay
MAT 4110/220	2 measuring circuits with 1 analog outputs each (not potentially separated against each other) and 1 limit value output OC each. The second measuring circuit can be activated with an activation code subject to costs.
MAT 4220	2 measuring circuits with 1 analog output each (not potentially separated against each other)*
MAT 4240	2 measuring circuits with 1 analog output each (potentially separated against each other)*

*) no change in software except type code)

2.1.1. mipromex type code:

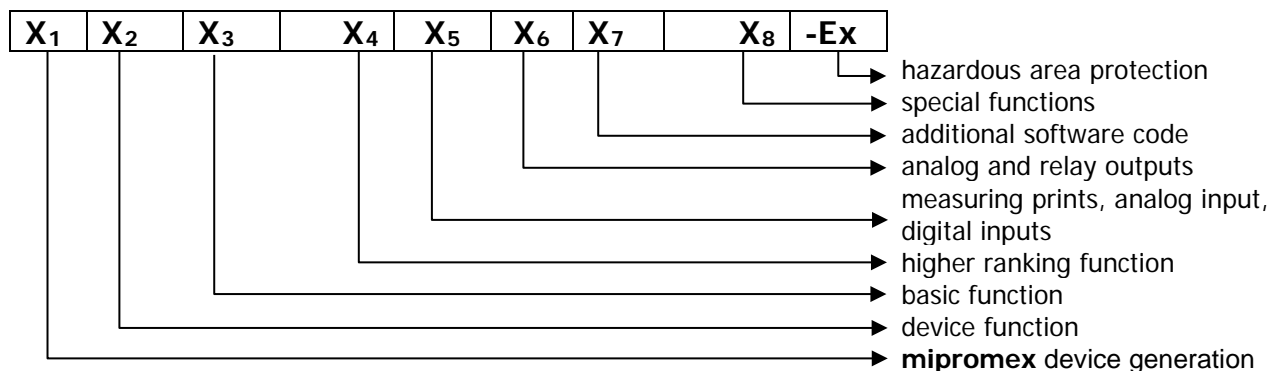

X₁ M = **mipromex**

X₂ A = Analog I = Interface
L = Level P = Product

X₃ L = Limit/Level M = Monitoring T = Transmitter
R = Recognition Q = Quality S = Switch
L = Level U = Universal

X₄ 1 = Limit switch 4 = Analog output 7 =
2 = Level switch empty 5 = Universal new 8 = Interfacial layer
3 = Level switch full 6 = Filling level 9 = Product (quality, type, concentration)

X ₅	Meas. print	MeV of 2nd. unit	analog input	digital input
1	1			3
2	2			3
3	2	1 MeV ex Rackbus		3
4	2	2 MeV ex Rackbus		3
5	1		1	3
6	2		1	3

X ₆	relay	OC	analog output	DC-converter
0	2			
1		1	1	1
2		2	2	1
3	2		1	1
4		2	2	2
5	2		1	1
6	2		2	1
7		2		
8	2 intern		1	1
9	1		1	1

One DC-converter, with potential separation, analog output toward power supply
Two DC-converter, additional potential separation, analog outputs toward each other

X₇ 0 = standard - software
1 = first expansion of a standard - software

X₈ - = without
C = controller (device with control function) e.g. **MIL 8110 C** interfacial layer level controller
P = product compensation
S = Segment

Ex Ex = with hazardous area protection according to ATEX II(2)G [Ex ia] IIC // II(2)D [Ex iaD]
Exd = with hazardous area protection according to ATEX II(2)GD [Ex d ia] IIC
NEEx = without hazardous area protection on measuring print

2.2. Software Versions

2.2.1. Basic

The standard operating software is used for all basic hardware units. The basic functions are identical for all software versions; you can use them on all the units. Software versions are marked according to NAMUR EN53.

Example:

MAT 419*	V1.1x	1 measuring circuit with one analog output and one Relay limit value
MAT 411*/22*	V1.1x	2 measuring circuits with 1 analog outputs each (not potentially separated against each other) and 1 limit value output OC each. The second measuring circuit can be activated with an activation code subject to costs.
MAT 422*	V1.1x	2 measuring circuits with one analog output each and one limit value each*
MAT 424*	V1.1x	2 measuring circuits with one analog output each (potentially separated against each other) and one limit value each*

(* no change in software except type code)

Within each software type, at cost, additional functions can be activated.

For each additional function a separate activation code is generated for each measuring circuit. The activation code is serial number depending.

Examples for additional functions:

- Second measuring circuit for **MAT 411*/422***

The simple menu navigation (language selectable) assures a fast and accurate operation.

Input can be made via buttons and display of the device or via connection to a laptop or the process control system.

2.3. Basic functions

The **mipromex MAT** has one or two separated and independent measuring circuits. Depending on the device type, one or two measured signal processing can be activated.

The pulse signal transmitted by the measuring electronic MTI is transformed into an offset compensated and filtrated pulse value and converted into a 4 – 20 mA signal in function of the selected measuring span.

The output signal is displayed as pulses value, % value or as mA value.

The offset range can be set between 10 and 2000 pulses.

The measuring signal offset (zero point) can be picked up automatically and/or the stored value can be modified via the keypad buttons. The measuring span is product dependent determined and automatically stored and/or the stored value can also be modified manually via the keypad buttons.

The pulses signal is converted into a 0 – 100 %-value.

The 4 - 20 mA analog output can be spread via programmable start and end values.

Parameter input is menu-driven and device-type based. Inactive positions are hidden.

The parameters can be stored and reloaded.

For each measuring circuit, an opto-electronic coupler transistor output (OC) with Low and Hi function as well as an adjustable time delay for drop and activation is at disposal. Fault messages are visualized with time and date of the error.

2.4. Measuring circuit

One or two probes with the measuring electronic MTI in the connecting head are connected to the **mipromex MAT** using a shielded two core cable. Between field and control room an equipotential bond must be installed.

2.5. Function

A product surrounding or filling an Aquasant-mt impedance pipe or bar probe you varied the impedance in function of the dielectrical constant and/or conductivity characteristics of organic products or aqueous solutions as, well as the immersion depth of the active part of the bar probe .

The measured impedance sum signal is converted directly by the measuring electronic MTI into a normed signal and is transmitted as pulse packages to the analog transmitter **mipromex MAT**.

The measured values within the normed signal range are product specific and characteristic for the different products and changing in accordance with product mixtures or immersion depth - This product specific measured value correspond to a value in the range of 0 – 3700. The physical impedance measured value of a product is registered in digits, designed as pulses value.

In a measuring electronic range (e.g. MTI 100) the dielectrical value of 100 pF is converted into a range of 0 – 3500 pulses.

A modern and menu driven operation and calibration concept enables a time saving commissioning of the analog transmitter. The frontal key pad with function and graphic display assure a user friendly operation and reliable working.


Use for foam and powder surveillance, recognition of water in petrochemical products or organic products in water or surveillance of surface oil layers with floater probes

2.1. Measured values processing

The safety level switch MLS is equipped with 2 different measured values processing modes: **stat** and **dyn**. The factory setting at delivery or after initialization is the **stat** (static) process mode.

Pos.-Nr.	settings	description
6.1.2	stat/dyn	Static measure processing mode
6.1.7	FSL/FSH	Safety level (full) switch


2.1.1. Static measure processing mode

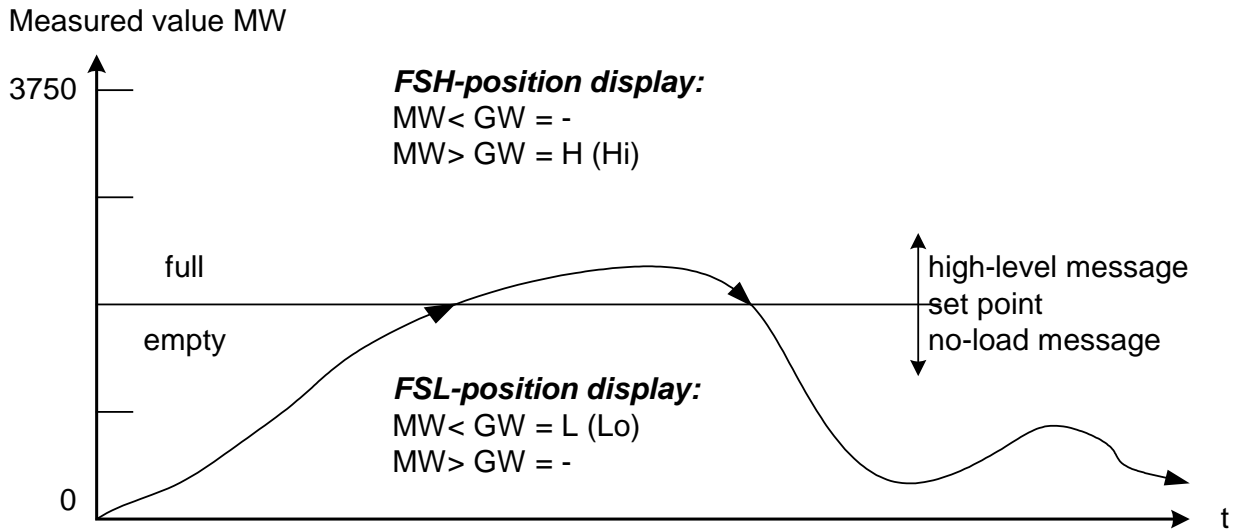

Pic. 2 static measure processing mode

2.1.2. Dynamic measure processing mode

Nr.	settings	description
6.1.2.	stat/ dyn	Dynamic measure processing mode
6.1.3.	3000 Imp	Max. limit value (as example below)
6.1.4.	50 Imp	Hysteresis (as example below)
6.1.5.	00.02 mm.ss	Relay Time delay, drop
6.1.6.	00.00 mm.ss	Relay Time delay, tension
6.1.7.	FSL/ FSH	Safety level (full) switch

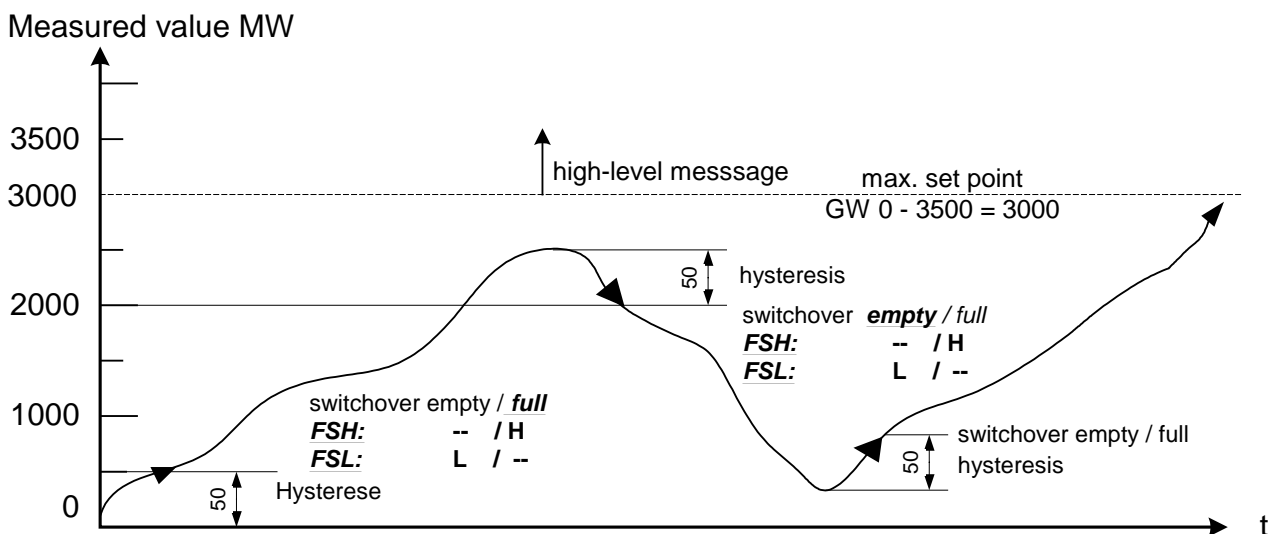

Pic. 3 dynamic processing mode

3. Structure of data input (parameterization)

3.1. General

To select a menu point or to go forward/ "next" step in the menu, use the **OK** button.

The function of the **OK** button is shown in the inversed bar at the bottom of the display.

The position number of the actual menu item is displayed at bottom left.

To select the desired menu item use the **▲ ▼** buttons. The selected menu item is shown inversed. To execute the shown function use the **ok** button, to delete a value or go back to the previous menu, use the **C** button.

3.2. Key functions

Key	description	Messwert-Anzeige	in main menu	menu line	Data input
▲	up	Advancing display	"next" menu item	1 step up	0 - 9 / A - Z
▼	down	next dysplai	"next" menu item	1 step down	0 - 9 / A - Z
▶	right	-	no function	no function	input right
◀	left	-	no function	no function	input left
OK	"next" / menu / select / store	(>2 s) Confirmation error	select	confirm	forward or (>2 s) store and forward
C	back	retour	back	back	back

Chart 2 Key functions

3.2.1. Input / changing of characters

Every parameter has its own input field.

The input and change of parameter values can be done using the **mipromex** menu or via PC-Software.

For several menu configuration text input is required. Text input is done the same way in all functions.

Input via buttons on the **mipromex** key pad is done as follows:

The first position, beginning on the left, is inverted. To change the character use the **▲ ▼** buttons.

To select the next position use the **◀ ▶** buttons.

With the **ok** button (press >2 sec) the new value is stored and the display changes to the next parameter.

You can reactivate the old value using the **C** button. If no input is made during an adjustable amount of time, the display changes back to measured value.

Define your position, instrument or tag-number, 11 characters max.

active key-navigation

Menu-Pos.-Nr.-Code / **ok** button function

Input Tag.-No.

1 Tag SR10P _ _ _ _ _

▲ ▼ ◀ ▶ adjust

3.1.1. Store

Change and input

1. position character input using ▲ ▼ buttons alpha-numerical

active button function

press **ok** key more than 2s; store and advance to the next Menu item

Chart 3 Display

3.2.2. Select language

The languages Deutsch/English/Français are available and selectable in the **mipromex** menu. A fourth language can be programmed. The parameter text field is loaded according to language code via PC-Software. Changes of the text can not be done using only the microprocessor unit **mipromex!**



3.3. Graphic display

The format of the display is as follows:

Every menu position, parameter and device unit can be set active or inactive (not visible) according to the function of the device. The display is also adjusted to the function of the device.

3.3.1. Display at switch-on of mipromex

Vendor	
Name of device generation	
ok button function	Next

ok: forward to device type

Unit description	Analog transmitter Device type MAT 4191
Device type and hardware model	
ok button function	Next

ok: forward to meas.value display

3.3.2. Measured value display

Unit type (with 1 measuring circuit) **MLS 1100, MAT 4191, MLT 6130, MIQ 8130, MIL 8110**

Description of the 1. measuring position	1 Pos. QLA12345 678 Analog output 1 100.0 % Hi Menu ▲▼	Change and input in measuring circuit 1, Menu 3.1.1.
Description of the (1 st) measured value		Limit value "Hi" (high) is reached
Actual calibrated meas.value display in %		Change and input in measuring circuit 1, Menu 6.1.2
Change and input in Menu 5.1.2		▲▼ : circulate (loop) in display mode

ok: change back to menu

Pos. no. can be entered in the menu

Unit types with 2 measuring circuits: **MLS 1200, MAT 4221/4241, MLT 6250, MIL 8240**

Description of the 2 nd measuring position	2 Pos. QLA12345 679 Analog output 2 100.0 % Hi Menu ▲▼	Change and input in measuring circuit 2, Menu 3.1.1.
Description of the 2 nd measured value		Limit value "Hi" (high) is reached
Actual calibrated meas.value display in %		Change and input in measuring circuit 2, Menu 6.1.2
Change and input in Menu 5.1.2.		▲▼ : circulate (loop) in display mode

ok: change back to menu

Description of the outputs	Analog outputs 1 100.0 % 2 100.0 % Menu ▲▼
Display of the 1 st and 2 nd measured value	
Actual calibrated meas. value display in %	
Change and input in Menu 5.1.2.	

ok: change back to menu

In case of alarm sign **▲**, "Lo" or "Hi" : no display of impulse or % values/digits

Description of the outputs	Analog outputs 1 20.00 mA 2 20.00 mA Menu ▲▼
Display of the 1 st and 2 nd measured value	
Display of actual current output values	
ok button function / active keys	

ok: change back to menu

▲▼ : circulate (loop) in display mode (loop)

Description of the 1st measuring position
 Display of the measured value
 Actual calibrated meas.value display in %
 measured value display in pulses

1 Pos. QLA12345 678

100.0 %

3750 Imp

Menu ▲▼

ok button function / active keys

ok: change back to menu ▲▼: circulate (loop) in display mode

Description of the 2nd measuring position
 Display of the measured value
 Actual calibrated meas.value display in %
 measured value display in pulses

2 Pos. QLA12345 679

100.0 %

3750 Imp

Menu ▲▼

ok button function / active keys

ok: change back to menu ▲▼: circulate (loop) in display mode

3.3.3. Menu parameter settings

After pressing the OK button the display changes to the info menu.

Menu-Information
 Both functions of the **ok** button
 store or
 next

=> Menu-Info <=

Press OK button

> 2s store !

< 2s next !

Info 01 Next

Menu Pos. No. / **ok** button function

ok: change to password input

After pressing the OK button the display changes to the password input.

selected character is inverted

Key in Password !

0000

▲▼◀▶ adjust

1. Store

Menu Pos. No. / **ok** button function

ok: change to the menu

1. key-in the numerical password using the ▲▼◀▶-buttons
 2. press **ok** button more than 2 seconds
 Standard factory password 0000
 Display changes to the menu
 Parameters can be changed

After pressing the OK button the display changes to the menu.

selected menu item is inverted

Basic settings

Device specs

Signal settings














































Measuring range

1. Select ▲▼

Menu Pos. No./**ok** function/active keys

ok: change to the selected menu item ▲▼: circulate (loop) menu items

4. Program structure with parameters of the analog transmitter

Legend:  = Select /  = Input /  = Display /  = only available with activation code		Type:	MAT 4191	MAT 4191/261	MAT 4261	MAT 4241	Change
Menu-Code Parameter							
1.	Basic settings		<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
1.1.	Language		<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
1.1.1.	Deutsch		<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
1.1.2.	English		<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
1.1.3.	Français		<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
1.1.4.	Free language / text		-	-	-	-	
1.2.	Time/Date		<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
1.2.1.	Time, input/correction		<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
1.2.2.	Date, input/correction		<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
1.3.	Modify Password		<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
1.3.1.	Password input		<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
1.3.2.	Modify password		<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
1.4.	Lighting		<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
1.4.1.	Lighting on/off		<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
1.4.2.	Duration of lighting in min. / 0 = continuous ON		<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
1.5.	Contact information		<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
1.5.1.	Contact address		<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
1.5.2.	Contact Tel./E-Mail		<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
1.5.3.	Contact Web		<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
1.6.	Factory settings		<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
1.6.1.	Store parameter set		<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
1.6.2.	Load parameter set		<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
1.6.3.	Initialize device no/yes		<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
1.7.	Activation code						
1.7.1.	Activation of 2 nd measuring circuit, Code: *****		-	<input checked="" type="checkbox"/>	-	-	
2.	Device specs		<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
2.1.	Device type: MAT 4190 or 4110/220 or 4220 or 4240 Software: Version V....		<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
2.2.	S/N and system verification date		<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
2.3.	Quantity of measuring circuits (1 measuring circuit: skips 2.4.0/3.1.0/4.1.0) Battery type: CR2032		<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
2.4.	Select measuring circuit 1 or 2		-	-	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
2.4.1.	Type code probe 1 / 2		<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
2.4.2.	S/N 1 / 2		<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
3.	Signal settings		<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
3.1	Select measuring circuit 1 or 2		-	-	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
3.1.1.	Input position number / TAG number		<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
3.1.2.	Probe factor		<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
3.1.3.	Zero point input (Offset), accept at press of OK button, store		<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	

Legend:							
= Select / = Input / = Display / = only available with activation code		Type:	MAT 4191	MAT 4191/261	MAT 4261	MAT 4241	Change
Menu-Code Parameter							
3.1.4.	Manual input of the zero point (Offset)	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>		
3.1.5.	Measuring span, accept at press button	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>		
3.1.6.	Height in percent at auto measuring span	-	-	-	-		
3.1.7.	Measuring span input / correction manual	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>		
3.1.8.	Signal filter	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>		
4.	Commissioning according to device type	-	-	-	-		
4.1	Select measuring circuit 1 or 2	-	-	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>		
5.	Measuring range	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>		
5.1	Select measuring circuit 1 or 2	-	-	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>		
5.1.2.	Measuring range starting point	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>		
5.1.3.	Measuring range end point	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>		
6.	Limit values	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>		
6.1	Select measuring circuit 1 or 2	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>		
6.1.1.	static/dynamic	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>		
6.1.2.	Limit value(s)	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>		
6.1.3.	Hysteresis /max. measured value	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>		
6.1.4.	Time delay, drop 1	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>		
6.1.5.	Time delay, tension 1	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>		
6.1.6.	FSL/FSH position	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>		
6.1.7.	Min./Max. measure value memory	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>		
7.	Test functions	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>		
7.1.	Select measuring circuit 1 or 2	-	-	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>		
7.1.1.	mA- output simulation (0.1 mA steps) beginning at 0.5 mA	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>		
8.	Error message mA output	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>		
8.1.	Data error, measured value underflow, <0010 pulses	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>		
8.2.	Data error, measured value overflow, >3750 pulses	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>		
8.3.	Technical error	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>		
	Display actual error with time/date	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>		
9.	Controller function	-	-	-	-		
10.	Protocol of active data set						
11.	Service parameter basic settings	-	-	-	-		
11.1.	Service parameter list (encoded)	-	-	-	-	PC	
11.2.	Parameter list for different device types						
12.	Calculation parameters	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>		
12.1.	Select measuring circuit 1 or 2	-	-	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>		
12.1.1	Drift memory	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>		
12.1.2	Drift gradient	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>		
13.	Archive						
13.1.	Operation parameter sets (last set of parameters)	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>		

Legend: = Select / = Input / = Display / = only available with activation code Menu-Code Parameter	Type:	MAT 4191	MAT 4111/221	MAT 4221	MAT 4241	Change

<i>Display modes</i>					
Analog output 1 in %	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
Analog output 2 in %	-	-	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
Analog output 1 in mA	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	-	-	
Analog output 1/2 in %	-	-	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
Analog output 1/2 in mA	-	-	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
1. Pos. Number analog output 1 in % and measured value in pulses	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
2. Pos. Number analog output 2 in % and measured value in pulses	-	-	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	
Display actual error with time /date	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	

Chart 4 Program structure

4.1. Description of the menu, program structure General, for all mipromex units



mipromex display



Your TAG or Position number
Measuring position, number
Display measured value in %
Hi = High Alarm

1 Pos. QLA12345678
Analog output 1
100.0 % Hi
Menu ▲▼

After pressing the **ok** button the display changes to the info menu.

ok button function / active keys

Information about storing or next

=> Menu-Info <=
Press OK button
>2s store !
< 2s next !
Info 01 Next

After pressing the **ok** button, the display changes to password input.

Password

The password protects the programming level of the **mipromex**. If you start up for the first time, the standard password is **0000** and is displayed. If you change the password (under point 1.3.) every user has to log-in using the new password!

Note: If you loose the new password, contact aquasant-mt to obtain an override password.

Key in your new password or accept the standard password
selected digit is inverted

Key in Password !
0000
1. Store

1. Key-in the numerical password using the ▲▼◀▶ buttons
2. Press **ok** button more than 2 seconds

Display changes to the menu
Parameters can be changed

4.1.1. [1.] Basic settings

You can set the device specific parameters in the basic settings menu. Please note that you first have to activate the password before you can make any changes.

Main menu
selected menu item is inverted

Basic settings
Device specs
Signal settings
Measuring range
1. Select ▲▼

After pressing the **ok** button the display changes to the sub menu basic settings

Sub menu
Selected sub menu item is inverted

Language / Sprache
Time/Date
Modify password
Lighting settings
1.1. Select ▲▼

After pressing the **ok** button the display changes to the sub menu Language / Sprache

[1.1.] Language/Sprache

Select the desired language. After you selected the language and stored your choice, the new language will be activated immediately. On the internet homepage www.aquasant-mt.com / Downloads, you can download an Excel-file. The three languages Deutsch, English and Français are listed. Replenish all text blocks in your language (max 16-characters), send it to us and we will be glad to implement your language.

selected menu item is inverted



Deutsch
English
Français
1.1.1 Store ▲▼



1. select language with the ▲▼-buttons
2. press **ok** button more than 2 seconds

The selected language is immediately activated
Display changes back to menu item 1.1.

[1.2.] Time/Date



Correction of device time and date. The time is displayed in hours, minutes and seconds. Daylight saving time is not adjusted automatically! The date is displayed in day, month and year. The device time is used for the protocol logger.

current time		<ol style="list-style-type: none"> 1. use ▲▼◀▶-buttons to change the time 2. press ok button more than 2 seconds
selected character is inverted		
active key-navigation		Time is stored
		Display changes to date 1.2.1.

current date		<ol style="list-style-type: none"> 1. use ▲▼◀▶-buttons to change the date 2. press ok button more than 2 seconds
selected character is inverted		
active key-navigation		Date is stored
		Display changes back to menu item 1.2.



[1.3.1.] Key-in and change password

The *standard password (0000)* can be changed. The old password has to be confirmed first.

selected character is inverted		<ol style="list-style-type: none"> 1. use ▲▼◀▶-buttons to input the numerical password 2. press ok button more than 2 seconds
		Password is stored
		Display changes to modify password 1.3.2.



[1.3.2.] Modify password

The standard password (0000) can be changed. The new password has not to be confirmed.

selected character is inverted		<ol style="list-style-type: none"> 1. use ▲▼◀▶-buttons to input the numerical password 2. press ok button more than 2 seconds
		New password is stored
		Display changes back to menu item 1.3.



[1.4.1.] Lighting

The display lighting can be switched on or off. The duration of the lighting can be set in minute-steps; for continuously on choose time 00, under the menu point 1.4.2.!

selected character is inverted		<ol style="list-style-type: none"> 1. use ◀▶-buttons to switch the lighting on or off 2. press ok button more than 2 seconds
		Selection is stored
		Display changes to sub menu lighting duration 1.4.2.

[1.4.2.] Lighting settings

The display lighting can be switched on or off. The duration of the lighting can be set in minute-steps; for continuously on choose 00!

selected character is inverted		<ol style="list-style-type: none"> 1. use ▲▼◀▶-buttons to select the lighting duration 2. press ok button more than 2 seconds
active key-navigation		
		Lighting duration is immediately activated
		Display changes back to menu item 1.4.

[1.5.] Contact

Our contact information: Address / Phone-No. / Email / Web

**Aquasant-mt
measuring tech. Ltd
Hauptstrasse 22
CH-4416 Bubendorf
1.5.1. Next**

After pressing the **ok** button the display changes to the next menu item.

/ **Switzerland**

**Tel.:
+41(0)61 9355000
Email: info@
aquasant-mt.com
1.5.2. Next**

After pressing the **ok** button the display changes to the next menu item.

/ **info@aquasant-mt.com**

**Web: www.
aquasant-mt.com
1.5.3. Next**

After pressing the **ok** button the display changes back to the sub menu Contact 1.5

/ www.aquasant-mt.com

[1.6.] Factory settings

Under the **Factory settings** Menu Level, the programmed device parameters can also be stored, reloaded or deleted. All parameters are set back to factory settings at initialization of the device.

[1.6.1.] Store Parameter set

All keyed-in parameters are stored in the flash memory of the unit. The parameters can be reloaded afterwards.

**Store parameter
ok
1.6.1. Store**

[1.6.2.] Load Parameter set

If parameters have been changed or deleted, the last flash stored parameter set can be reloaded into the RAM.

**Load parameter
ok
1.6.2. confirm**

[1.6.3.] Initialize unit no/yes

If the device is initialized, all user-programmed parameters are deleted and set back to factory settings.

**Initialize unit
no/yes
1.6.3. confirm**

[1.7.] Activation code

With the activation code, several optional dutiable *software packages/functions* can be activated. You can obtain the activation code by ordering the optional packages/functions (e.g. *MK 220* Article-No.: 02.05.03.0019). The activation code is *depending on the serial-number* and can not be used for other devices.

[1.7.1.] Activation of/for 2nd measuring circuit

On the Hardware type **MAT 4110/220** with one active measuring circuit, the second measuring circuit can be activated. If the code is entered incorrectly the menu jumps back to menu item 1.7. The code can be entered again! Once the second measuring circuit is activated, it can not be deactivated. At start-up the new hardware type **MAT 4220** will be displayed.

<p>Description</p> <p>Code input</p> <p>active key-navigation</p>	<p>Activation for 2nd meas. circuit, code: xxxxxxxxxxxxxxxx ▲▼◀▶ Adjust 1.7.1 Store</p>	<p>1. use ▲▼◀▶-buttons to input the alpha-numerical Code</p> <p>2. press ok button more than 2 seconds</p> <p>Input is stored Display changes back to menu 1.</p>
---	--	---

4.1.2. [2.] Device specs

In the device specs you will find specific information about the **mipromex**.

<p>Main menu</p> <p>selected menu item is inverted</p>	<p>Basic settings</p> <p>Device specs</p> <p>Signal settings</p> <p>Measuring ranges</p> <p>2. Select ▲▼</p>	<p>After pressing the ok button the display changes to the sub menu Device specs</p>
--	---	---

[2.1.] Device type MAT 4190 or 4110/220 or 4220 or 4240

In the device type menu the hardware type and the software-release are displayed. Example:

- MAT 4191** with 1 measuring circuit (activation code 1.7.1. inactive)
- MAT 4191/261** with 2 measuring circuits, but only one is activated (activation code 1.7.1.)
- MAT 4261** with 2 active measuring circuits
- MAT 4241** with 2 active measuring circuits, plus analog outputs galvanically separated against each other

Software versions are marked according to NAMUR EN53. (V 1.00)

<p>Device type: MAT4191 Software: V1.1x 2.1. Next</p>	<p>After pressing the ok button the display changes to the next menu item 2.2.</p>
--	---

[2.2.] Serial number and date of the system verification

The serial number is fix stored in the **mipromex** and can not be changed. The serial number is linked to the activation codes. The date of the system verification marks the QS-function control during the final function test.


<p>Serial number: 42200001-07 Verification date: 10.12.07 2.2. Next</p>	<p>After pressing the ok button the display changes to the next menu item 2.3.</p>
--	---

[2.3.] Number of measuring circuits (1. measuring circuit, skip 3.1/4.1)

Here is displayed if there is one or two measuring circuits activated.

Battery type

The inserted battery type is displayed. The battery has not to be charged before using the **mipromex**. The battery lifetime of 10 years guarantees that no data loss will occur.

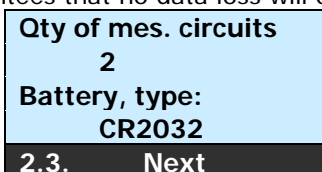


After pressing the **ok** button the display changes to the next menu item 2.4.

[2.4.] Select measuring circuit 1 or 2

Select the active measuring circuit for the next steps.

selected menu item is inverted

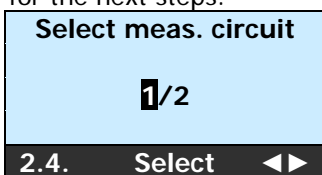


After pressing the **ok** button the display changes to the menu of the selected measuring circuit (1). 2.4.1.

[2.4.1.] Probe Type 1 / 2

This is an input field. If the system is delivered with a probe, the probe type is stored here.

selected character is inverted 16-char. max

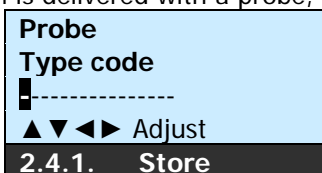

1. use ▲▼◀▶-buttons to input the alpha-numerical type code of the probe
2. press **ok** button more than 2 seconds

Type code is stored
Display changes to the next menu item 2.4.2.

[2.4.2.] Serial No. 1 / 2

This is an input field. If the system is delivered with a probe, the serial no. of the probe is stored here.

selected character is inverted 16-char. max



1. use ▲▼◀▶-buttons to input the alpha-numerical serial number of the probe
2. press **ok** button more than 2 seconds


Serial number is stored
Display changes back to menu 2.4.

4.1.3. [3.] Signal settings

In the signal settings menu all signal related parameters can be set.

Main menu

selected menu item is inverted

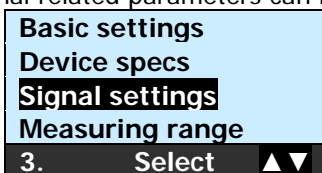


After pressing the **ok** button the display changes to the sub menu signal settings

[3.1.] Select measuring circuit 1 or 2

Select the active measuring circuit for the next steps.


selected menu item is inverted

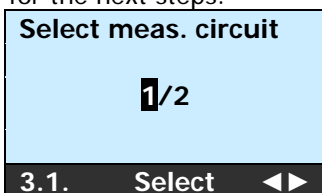

After pressing the **ok** button the display changes to the menu of the selected measuring circuit (1). 3.1.1.

[3.1.1.] Input Pos. No.

You have the possibility to store a Tag No. for the probe in the **mipromex**. The field is alphanumerical. You can define your position- or Tag-number, 11-characters max. The selected character is inverted

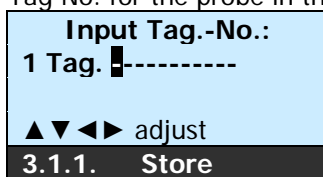


1. use ▲▼◀▶-buttons to input the alpha-numerical position number
 2. press **ok** button more than 2 seconds
- Pos.-No. is stored
Display changes to menu item 3.1.2.

[3.1.2.] Probe factor

The probe factor is a probe specific number which indicates the correlation to the standard probe (factor 1.00). If you replace the probe you will get a reproducible measurement with the same measured values. The probe factor has only to be changed when using a replacement probe. By changing the factor, you will get with the replacement probe, the same pulses value at 100 %

e. g. MeV old probe 2600 / 2955 MeV new probe = f 0.879

The probe factor has only to be changed when using a replacement probe selected character is inverted

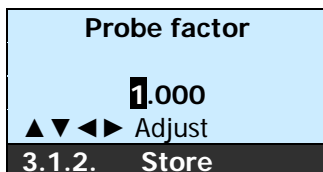


1. use ▲▼◀▶-buttons to define the probe factor
 2. press **ok** button more than 2 seconds
- Probe factor is stored
Display changes to the next menu item 3.1.3. After changing the probe factor the zero point must be actualized and stored 3.1.3.

[3.1.3.] Zero point acceptance at push button (Offset) OK store

The probe electronic is calibrated in the factory to 60 ±2 pulses. If the probe is installed, this value can be higher due to the environment. If the probe is installed; empty and dry, the zero point can be checked and/or manually corrected. Attention: switch-on the unit 30 minutes before the zero adjust. A measured value between 10 and 2000 pulses can be adjusted without performing an electronic calibration. **Attention; Probe must be dry and clean!**
MeV = normed measured value in pulses

actual stored zero point offset
actual raw measured value, empty probe

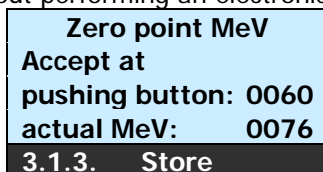


1. press **ok** button more than 2 seconds
- The new zero point is immediately activated
Display changes to the next menu item 3.1.4.

[3.1.4.] Manual zero point input (offset)

The programmable probe zero point can be changed or corrected manually. If the installation cannot be emptied for the zero point of the probe, then the zero point is manually keyed-in from the protocol

You can manually correct the zero point of the probe
actual raw measured value of the probe
adjust zero point

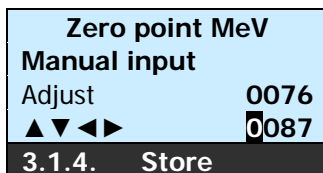


1. use ▲▼◀▶-buttons to define the zero point
 2. press **ok** button more than 2 seconds
- The new zero point is immediately activated
Display changes to the next menu item 3.1.5.

[3.1.5.] Measuring span acceptance at push button

The measuring span for the calculation of the 100 % point is product depending. This pulses value is obtained by fully immersing the measuring electrode into the product and by saving "at push button" the measured value. **Attention: this procedure is in dependence of point 3.1.6.**

MS = normed measuring span in pulses
actual stored measuring span
(raw measured value – zero point offset)

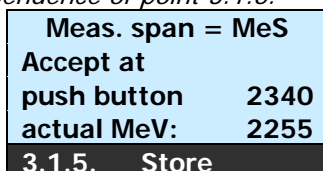


1. press **ok** button more than 2 seconds
- The new measuring span is immediately activated
Display changes to the next menu item 3.1.7.

[3.1.7.] Measuring span

The measuring span (point 3.1.5) can be changed or corrected here manually.

You can manually correct the Measuring span of the probe
actual measured value of the probe
Adjust measuring span

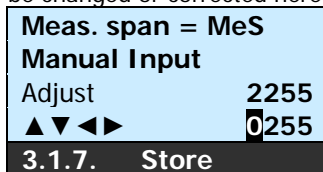


1. use ▲▼◀▶-buttons to define the measuring span
 2. press **ok** button more than 2 seconds
- The new measuring span is immediately activated
Display changes to the next menu item 3.1.8.

[3.1.8.] Signal filter

With the free selectable filter time constant (max 30 seconds) you can attenuate the raw measuring signal. A way to center the displayed and power output values

Input the filter constant
filter of the first order
actual stored filter constant

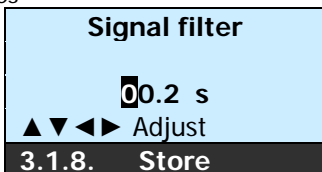


1. use ▲▼◀▶-buttons to define the signal filter time
2. press **ok** button more than 2 seconds

The new time is immediately activated
Display changes back to menu 3.1.

4.1.4. [5.] Measuring range

In the measuring range menu all measuring range related parameters can be set.

Main menu
selected menu item is inverted

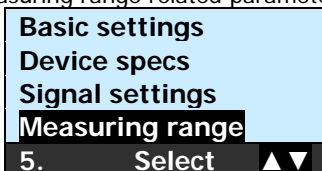


After pressing the **ok** button the display changes to the sub menu measuring range 5.1.

[5.1.] Select measuring circuit 1 or 2

Select the active measuring circuit for the next steps.

selected menu item is inverted

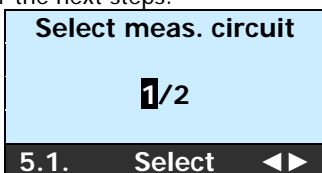


After pressing the **ok** button the display changes to the selected measuring circuit menu (1). 5.1.2

[5.1.2.] Measuring range starting point

Set the start point of the selected measuring range (e.g. 20.0 – 60.0 %). By defining the start and the end point you can *spread* the mA signal and therefore get a higher resolution in this area.

selected character is inverted

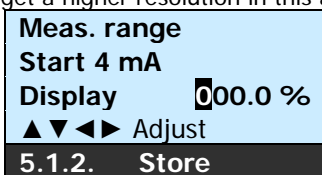

1. use ▲▼◀▶-buttons to define the start point
2. press **ok** button more than 2 seconds


The new spreading is immediately activated

Display changes to the next menu item 5.1.3.

[5.1.3.] Measuring range end point

Set the end point of the selected measuring range (e.g. 20.0 – 60.0 %)

selected character is inverted

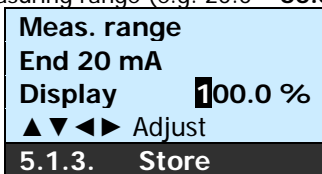

1. use ▲▼◀▶-buttons to define the end point
2. press **ok** button more than 2 seconds


The new spreading is immediately activated

Display changes back to menu 5.1.

4.1.5. [6.] Limit value

In the limit value menu all limit values related parameters can be set.

Main menu
selected menu item is inverted

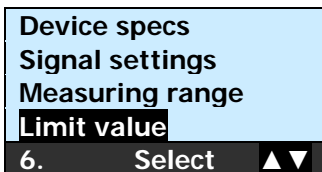


After pressing the **ok** button the display changes to the sub menu measuring ranges 6.1. select measuring circuit.

[6.1.] Select measuring circuit 1 or 2

Select the active measuring circuit for the next steps.

selected menu item is inverted

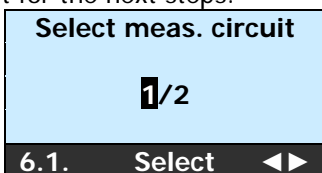

After pressing the **ok** button the display changes to the selected measuring circuit menu (1). 6.1.2

[6.1.1.] Select static or dynamic

With the static limit value you can:


- obtain a precise and reproducible limit value for a given measuring range corresponding to 100 %
- read a chosen limit value as a percentage and programme it as a limit value
- enter very small limit values, starting at 1.1 %, thanks to the high performance measuring circuit and the precise and reproducible processing of the measurement values

With the dynamic limit value you can:

- detect the limit value inside the length of the active measuring electrode independently of the product's properties and its adherence to the measuring electrode
- only one dynamic limit value should be set for each measuring circuit.
- see diagram for the processing of the measurement value

Diagramm (look on Capitel 2.6)

selected character is inverted

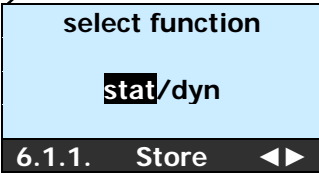

1 Use ▲▼◀▶-buttons to define the function
2. Press **ok** button more than 2 seconds


After pressing the **ok** button, the display changes to the menu Enter limit value or max limit value and hysteresis

[6.1.2.] Limit value

With the static limit value you:

- get an exact and reproducible limit value for a defined measuring span corresponding to 100 %
- can display read a desired percentage at the desired limit value and program it/store it, as limit value
- can enter exact limit values starting at 1.1% thanks to the precise and reproducible measuring values.

selected character is inverted

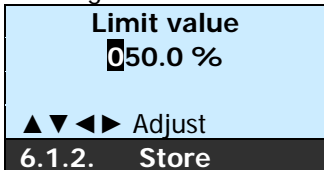

1. use ▲▼◀▶-buttons to define the limit value
2. press **ok** button more than 2 seconds


The selected limit value is immediately activated
Display changes to the next menu item 6.1.4.

Or wen your select dyn...

[6.1.2.] max. Limit value

After entering Dynamic

selected character is inverted

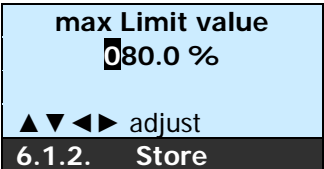


1. Use ▲▼◀▶-buttons to define the limit value
2. press **ok** button more than 2 seconds

The selected limit value is immediately activated
Display changes to the next menu item 6.1.4.

[6.1.3.] Hysteresis

After entering Dynamic

selected character is inverted

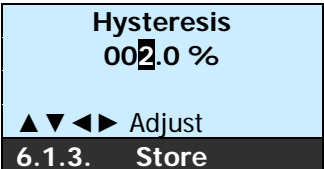


1. Use ▲▼◀▶-buttons to define the hysteresis
2. Press **ok** button more than 2 seconds

After pressing the **ok**-button display changes to the next menu item 6.1.4.

[6.1.4.] Time, drop down delay, 1

The relay- or opto-electronic coupler- transistor- output can be activated with a drop down time delay. Input of the time delay drop, in 1 second steps from 0 - 30 minutes.

selected character is inverted

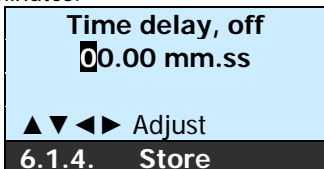


1. use ▲▼◀▶-buttons to define the time delay off, drop
2. press **ok** button more than 2 seconds

The selected time delay is immediately activated
Display changes to the next menu item 6.1.5.

[6.1.5.] Time, on delay, 1

The relay- or opto-electronic coupler- transistor- output can be activated with an on/raise time delay. Input of the time delay, of raise, in 1 second-steps from 0 - 30 minutes.

selected character is inverted

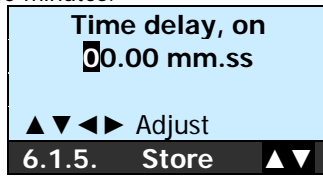

1. use ▲▼◀▶-buttons to define the time delay on, raise
2. press **ok** button more than 2 seconds

The selected time delay is immediately activated
Display changes to the next menu item 6.1.6.

[6.1.6.] FSL/FSH Position

Define the security settings of the Relay- or opto-electronic-coupler- transistor- outputs, ...

Active position	Measured value	Display	opto-electronic coupler
Fail Safe Low	is lower than limit value	Lo	de-energized
Lo-Alarm			
Fail Safe High	is higher than limit value	none	switched on
HI-Alarm			

Chart 5 Fail Safe settings


selected menu item is inverted



1. use ◀▶-buttons to define the opto-electronic coupler-output
2. press **ok** button more than 2 seconds

The selected definition is immediately activated
Display changes back to menu item 6.

[6.1.7.] min/max Measurement value

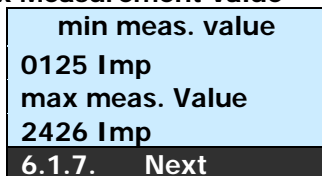


After pressing the **ok** button the display changes to the sub menu test functions 6.1. select measuring circuit

4.1.6. [7.] Test functions

To test the functions at commissioning, a programmable mA output is available.

Main menu

selected menu item is inverted

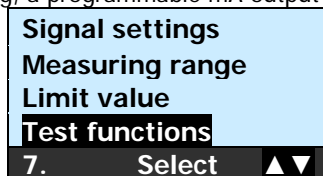


After pressing the **ok** button the display changes to the sub menu test functions 7.1. select measuring circuit

[7.1.] Select measuring circuit 1 or 2

Select the active measuring circuit for the next steps.

selected menu item is inverted

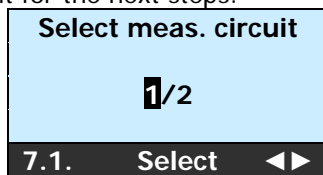

After pressing the **ok** button the display changes to the selected measuring circuit menu (1). 7.1.1

[7.1.1.] Simulation of mA- output (in 0.1 mA steps, starting at 0.5 mA)

With this function the active current output (burden 750 Ω) can be tested.

The current output can be increased in 0.1 steps starting at 0.5 mA and ending at max. 22.0 mA.

selected character is inverted




1. use ▲▼◀▶-buttons to define the current output
2. press **ok** button more than 2 seconds

Current output is immediately activated
Display changes back to 7.1.

4.1.7. [8.] Programmable mA output


All **mipromex** microprocessor units are equipped with a diagnostic system, which makes fault-finding easier and facilitates quicker correction in case of malfunction occurrence. The error levels can be set in 0.1 mA-steps between 0.5 - 4.0 and 20.0 - 22.0 mA. Error messages are set at factory to automatically acknowledge the fault. The fault-type is displayed with time and date. By pressing > 2 seconds the **ok** button, the display changes back to the measured value. The error is displayed without measured value ---.- and an arrow up ↑ or down ↓ .

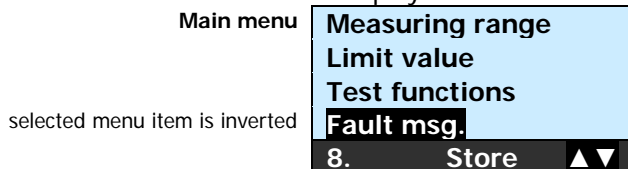

After pressing the **ok** button the display changes to the sub menu fault messages 8.1.

[8.1.] Data error measuring value underflow MeV <0010

The data transmission of the measured value, between measuring electronic MTI and the control unit **mipromex** is faulty. The control unit **mipromex** is unable to process the measured data. Error level 1 see fault finding on page 32

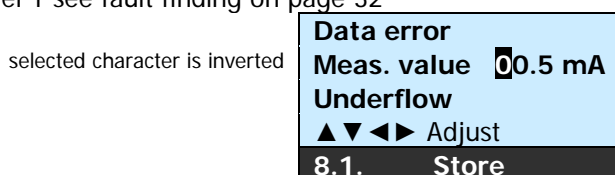


1. use ▲▼◀▶-buttons to define the current output
2. press **ok** button more than 2 seconds

Current output is immediately activated
Display changes to the next menu item 8.2.

[8.2.] Data error measuring value overflow MeV >3750

The measured value of the measuring electronic MTI is higher than the allowed range of pulses. The control unit **mipromex** is unable to process the measured data. Error level 2 see fault finding on page 32

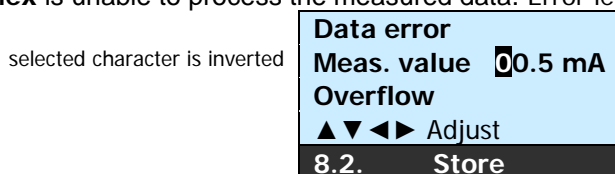


1. use ▲▼◀▶-buttons to define the current output
2. press **ok** button more than 2 seconds

Current output is immediately activated
Display changes to the next menu item 8.3.

[8.3.] Technical Error


The control unit **mipromex** generates a periodic checksum test. If it is faulty, an error message is displayed. Error level 3 see fault finding on page 32

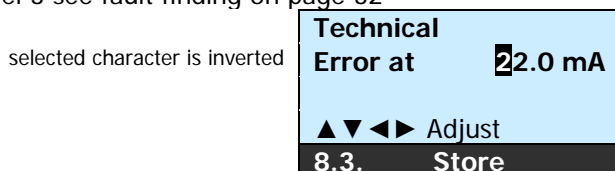

1. use ▲▼◀▶-buttons to define the current output
2. press **ok** button more than 2 seconds

Current output is immediately activated
Display changes back to menu 8.

4.1.1. [12.] Calculation parameters

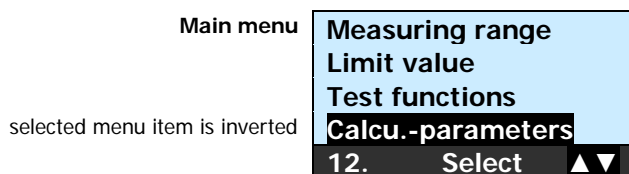

After pressing the **ok** button the display changes to the sub menu 12.1. select measuring circuit

[12.1.] Select measuring circuit 1 or 2 (MLS 1200/1270)

With the drift compensation small measurement modifications like temperature drift are compensated for by HF wire or probes. ± 1-3 impulses per minute correspond to normal drift compensation. With the drift compensation the measurement has left constantly if the drift is smaller than the drift gradient. This means the measurement corrects itself the max. drift in impulses is fixed in the drift memory within a minute (adjusting drift time 60 s). The sum of the individual drift compensations becomes e.g. 30 (impulses) to change the measurement more greatly than 30 impulses begin itself into function of the drift. At a zero comparison [3.1.3.] the drift loft is put on 0000. Around min. 40 impulses, the zero comparison must always be GREATER than Max Driftspeicher. The measurement otherwise sinks at a negative drift under the zero. Consequence is: Technical disturbance measurement underrun!

At the measuring of at times slow modifications like filling level measuring the drift compensation must get prepared for 0 Imp, i.e. turned off.

Caution: With the drift compensation no probe pollutions can be compensated for.

Select the measuring circle for the further action.

selected menu item is inverted

Select meas. circuit

1/2

12.1. Select ◀▶

After pressing the **ok** button, display changes to the menu for the measuring circuit selected (1). 12.1.1.

[12.1.1.] Drift memory

selected menu item is inverted

drift

actual 212 Imp

max. 500 Imp

▲▼◀▶ Adjust

12.1.1. Store

1. use ▲▼◀▶-buttons to define max. drift
 2. press **ok** button more than 2 seconds
 +- drift

If the max. drift is exceeded, no more drift compensation is possible

[12.1.2.] Driftgradient pulses

selected menu item is inverted

drift pulses

000 Imp

▲▼◀▶ Adjust

12.1.2. Store

1. use ▲▼◀▶-buttons to define max. drift pluses
 2. press **ok** button more than 2 seconds
 +- drift

If the max. drift is exceeded, no more drift compensation is possible

[12.1.3.] Driftgradient time

selected menu item is inverted

drift time

0100 s

▲▼◀▶ Adjust

12.1.3. Store

1. use ▲▼◀▶-buttons to define max. drift time
 2. press **ok** button more than 2 seconds
 +- drift time

If the max. drift is exceeded, no more drift compensation is possible

5. Commissioning example

Make sure the connections in the Monorack or 19"-Rack are wired correctly and the probe is connected.
 The control unit **mipromex** is installed in the Rack and under tension.
 The green or red LED inside the MTI (measuring electronic) of the probe is lit.
 The vessel is empty; the probe is dry and clean.
 Follow the steps of the commissioning:

5.1. Commissioning the mipromex with a pipe probe

5.1.1. Detection of water in petrochemical products

The pipe probe is installed in the pipeline. The pipeline must be empty!

Menu-Code	Description	Example		Input
2.4.1	Check the probe type	TSS90 DN50		
2.4.2	Check the serial no. of the probe	1050066-06		
3.1.1.	Enter your TAG-, position- or measuring site- number	LS1200		
3.1.2.	Check the probe factor Only to be changed when using a replacement probe	1.000		
3.1.3.	Accept the actual zero point Important: the pipeline must be empty, Important: the pipe probe must be dry and clean Pipe probes are calibrated in the factory to 60 pulses If the probe is already product, please keep the factory settings	ideal between 60 – 80		
3.1.5.	Accept measuring span MS: Fill the pipeline with your petrochemical product with the highest water content The MS is product and nominal diameter depending	5 % water in paraffin oil MS 860 Imp = 100 %	paraffin oil 110 Imp = 12.5 %	
5.1.2.	Define the start point of the signal spread at 4 mA	instead of 0.0 %	new at 10.0 %	
5.1.3.	Define the end point of the signal spread at 20 mA	instead 100.0 %	new at 80.0 % = 4 % water	

Chart 6 Commissioning of water detection

5.1.2. Oil detection in process- or rain-water

The pipe probe is installed in the pipeline. The pipeline must be empty!

Menu-Code	Description	Example		Input
2.4.1	Check the probe type	TSS90 DN50		
2.4.2	Check the serial no. of the probe	1050066-06		
3.1.1.	Enter your TAG-, position- or measuring site- number	LS1200		
3.1.2.	Check the probe factor Only to be changed when using a replacement probe	1.000		
3.1.3.	Accept the actual zero point Important: the pipeline must be empty Important: the pipe probe must be and clean Pipe probes are calibrated in the factory to 60 pulses If the probe is already soiled with product, please keep the factory settings	ideal between 60 – 80		
3.1.5.	Accept measuring span MS: Fill the pipe with your process water The MS depends on the product and the nominal diameter	water MS 2570 Imp	5 % oil in water 2050 Imp	
5.1.2.	Define the start point of the signal spread at 4 mA	instead of 0.0 %	new at 80.0 %	
5.1.3.	Define the end point of the signal spread at 20 mA	instead 100.0 %	remains at 100.0 %	

Chart 7 Commissioning of oil detection

5.2. Commissioning the mipromex with a bar probe

5.2.1. Oil detection in process- or rain-water with float

Bar probe is installed and adjusted in the float. The bar probe must be dry and clean!

Menu-Code	Description	Example		Input
2.4.1	Check the probe type	STM 180/100 SB R TN ES SW V		
2.4.2	Check the serial no. of the probe	1050066-06		
3.1.1.	Enter your TAG-, position- or measuring site- number	LS1200		
3.1.2.	Check the probe factor Only to be changed when using a replacement probe	1.000		
3.1.3.	Accept the actual zero point Important: the bar probe must be dry and clean If the probe is already soiled with product please keep the factory settings	ideal between 60 – 80		
3.1.5.	Accept measuring span MS: Bar probe is 100 % immersed in your process water Accept the measured value as measuring span Probe 100 mm in water = 100% Probe 80 mm in water and 20 mm in oil	100 mm water 2700 Imp = MS = 100%	80 mm water 20 mm oil 2200 Imp = 81 %	
5.1.2.	Define the start point of the signal spread at 4 mA	instead of 0.0 %	new at 80.0 %	
5.1.3.	Define the end point of the signal spread at 20 mA	100.0 %	remains at 100.0 %	

Without an oil layer at surface of water, the display shows 100% = 20.0 mA
Chart 8 Commissioning of oil layer detection

5.2.2. Foam detection



Attention:

A limit switch detection of the top of the foam is a relative measurement.
Due to varying structure and consistence, and foam plus product variations, the measurement can not be considered as a filling level measure.

Bar probe is installed in the vessel. The bar probe must be dry and clean!


Code	Description	Example		Input
2.4.1	Check the probe type	ST2M 500/300 SB T2R GS DN50 C		
2.4.2	Check the serial no. of the probe	1050066-06		
3.1.1.	Enter your tag-, position- or measuring site-number	LS1200		
3.1.2.	Check the probe factor Only to be changed when using a replacement probe	1.000		
3.1.3.	Accept the actual zero point Important: the bar probe must be dry and clean If the probe is already soiled with product, please keep the factory settings	ideal between 60 – 80		
	If the measured value shows > 400 an electronic calibration is recommended Point 5.3 page 29 Otherwise the measuring span MS is limited			
3.1.5.	Accept measuring span MS: Immerse the probe 100 % in your foam and accept the measuring span If the probe is not fully immersed, the measuring span must be calculated to 100 % and keyed-in at menu item 3.1.7.	Full range 1270 Imp	50 % 635 Imp	
5.1.2.	Define the start point of the signal spread at 4 mA	0.0 %	remains at 0.0 %	
5.1.3.	Define the end point of the signal spread at 20 mA	100.0 %	remains at 100.0 %	
6.1.2.	max. Limit value	80 %		
6.1.3.	Limit switch detection by hysteresis	10 %		
6.1.4	Time, drop down delay, 1	00.02		

Chart 9 Commissioning of foam detection

5.3. Electronic calibration MTI, basic equalization

An electronic calibration has only to be done at following occurrences:

- ☑ Probes without reference electrode, flexible- or flat-probes where the *measured value* inside the *empty* vessel is smaller than 10 or bigger than 200
- ☑ After exchange of the measuring electronic MTI, or of the coax cable, or of the probe, or after repair of the probe
- ☑ If the zero adjust is not possible: displayed measured value >2000 or <10



Tip:


Adjust the measuring electronic MTI between 60 and 80 pulses
This allows the biggest possible measuring span of up to max. 3750 pulses.

Soiled or uncleaned probes should not be adjusted with an MTI calibration.



Probe dry and clean, built in the vessel

Go to the menu point 3.1.3.



Calibration of MTI as follows:
Using a screwdriver size No. 1, fine adjust to switch point of the LED from red to green (red will flicker).
Display between 60 and 80

The 0-point has been stored at the system test. If the probe is built in, dry and empty the 0-point can be checked and corrected.

Menu position Number-Code

Zero point MeV	
Accept at	
push button	0060
actual MeV	0085
3.1.3. Store	

change to the next menu item by pressing the **Ok** button

1. press **ok** button more than 2 seconds:

actual MeV is stored
Display changes to the next parameter input

Chart 10 Electronic calibration operating sequences

5.4. Inspection release of the parameters

Operating parameters (settings at final inspection on site at commissioning)

Company _____	Order _____
Building _____	PO no. _____
Plant _____	Project no. _____
mipromex MLS V1.12 Ex ia <input type="checkbox"/> Exd <input type="checkbox"/> Non-ex <input type="checkbox"/> Serial no. _____	
Measuring circuit 1	Pos./Tag no. _____
Probe type _____	Serial no. _____
Coax cable _____ Serial no. _____ MTI _____	Serial no. _____
Measuring circuit 2	Pos./Tag no. _____
Probe type _____	Serial no. _____
Coax cable _____ Serial no. _____ MTI _____	Serial no. _____

Chart for operating settings

Menu item	Meas. circuit	Description	Final inspection	Commissioning
1. Basic settings				
1.1.		Language Deutsch/Français/English	English	
1.2.1.		Time	Local time	Local time
1.2.2.		Date	Local date	Local date
1.3.1.		Password	0000	
1.4.1.		Lighting	on	
1.4.2.		Lighting time in minutes	1	
1.6.1.		Store the parameters	OK <input type="checkbox"/>	OK <input type="checkbox"/>
1.6.2.		Load the parameters	press OK button >2s	
1.6.3.		Initialize the device		Yes <input type="checkbox"/>
1.7.1.		Activation for the 2nd measuring circuit		
2. Device data				
2.1.		Device type Software version	MLS V1.12	MLS V
2.2.		Serial no. Testing date		
2.3.		Number of measuring circuits / Battery type: CR2032		
2.4.1.	MC1	Probe type		
2.4.2.	MC1	Probe serial no.		
2.4.1.	MC2	Probe type		
2.4.2.	MC2	Probe serial no.		
3. Signal settings				
3.1.1.	MC1	Entry of position/TAG no.		
3.1.2.	MC1	Probe factor	1.000	
		<i>Zero adjustment for tube/bar probe empty/clean</i>		
3.1.3./4.	MC1	Zero point importing on keystroke / manual entry	Imp	
3.1.5./7.	MC1	Measuring span importing on keystroke / manual entry / adjustment	Imp	
3.1.8.	MC1	Signal filter	s 00.1	
3.1.1.	MC2	Entry of position/TAG no.		
3.1.2.	MC2	Probe factor	1.000	
		<i>Zero adjustment for tube/bar probe empty/clean</i>		
3.1.3./4.	MC2	Zero point importing on keystroke / manual entry	Imp	
3.1.5./7.	MC2	Measuring span importing on keystroke / manual entry / adjustment	Imp	
3.1.8.	MC2	Signal filter	s 00.1	
5. Measuring ranges				
5.1.1.	MC/DO1	Measuring range unit		

5.1.1.	MC/DO2	Measuring range unit		
6. Limit values				
6.1.2.	MC1/DO1	Selection: stat / dyn		
6.1.3.	MC1/DO1	Set limit value 1 / (max. limit value → dyn)	%	
6.1.4.	MC1/DO1	Hysteresis (→ dyn)	Imp	
6.1.5.	MC1/DO1	Time delay, off	mm.ss	00.00
6.1.6.	MC1/DO1	Time delay, on	mm.ss	00.00
6.1.7.	MC1/DO1	FSL / FSH position		FSL
6.1.8.	MC1/DO1	min/max limit value display (→ dyn)		
6.1.1.	MC1/DO2	Selection: Limit value / Fault message → MLS 1100 / 1101 / 1170 only		
6.1.2.	MC2/DO2	Selection stat / dyn		
6.1.3.	MC2/DO2	Set limit value 1 / (max. limit value → dyn)	%	
6.1.4.	MC2/DO2	Hysteresis (→ dyn)	Imp	
6.1.5.	MC2/DO2	Time delay, off	mm.ss	00.00
6.1.6.	MC2/DO2	Time delay, on	mm.ss	00.00
6.1.7.	MC2/DO2	FSL / FSH position		FSH
6.1.8.	MC2/DO2	min/max limit value display (→ dyn)		
7. Test functions				
7.1.3.	MC1/DO1	Limit value 1 simulation OFF/ON	<input type="checkbox"/> i.O.	<input type="checkbox"/> i.O.
7.1.4.	MC2/DO2	Limit value 2 simulation OFF/ON	<input type="checkbox"/> i.O.	<input type="checkbox"/> i.O.
8. Fault messages				
8.1.		Actual fault with time/date		
12. Calculation parameters				
12.1.1.	MC1	Maximal drift storage in pulses	Imp	0100
12.1.2.	MC1	Drift pulses per time unit	Imp	0
12.1.3.	MC1	Drift time	s	0060
12.1.1.	MC2	Maximal drift storage in pulses	Imp	0100
12.1.2.	MC2	Drift pulses per time unit	Imp	0
12.1.3.	MC2	Drift time	s	0060
1.6.1.		Storing the parameters	OK <input type="checkbox"/>	OK <input type="checkbox"/>

Final inspection carried out by:

Commissioning carried out by:

Aquasant Messtechnik AG / Bubendorf /

6. Fault finding


All **mipromex** –microprocessor units are equipped with a diagnostic system, which makes fault finding easier and facilitates quicker correction in case of malfunction occurrence.

6.1. After power on

7.1.1. Technical error; All oder Nv Init from Flash oder low Battery


The error message can have different origin.

1. RAM memory check has failed

Date of error	02.11.08
Time of error	16:11:10
Error description	 Nv Init from Flash


1. press **ok** button more than 2 seconds, the error is confirmed and the display changes back to last active menu point

2. Flash memory check has failed

Date of error	02.11.08
Time of error	16:11:10
Error description	 All Init from Flash

1. press **ok** button more than 2 seconds, the error is confirmed and the display changes back to last active menu point

3. Battery is discharged and has to be exchanged

Date of error	02.11.08
Time of error	16:11:10
Error description	 Low Battery

1. press **ok** button more than 2 seconds, the error is confirmed and the display changes back to last active menu point

Switch OFF and then switch ON the unit. If error reoccurs then:


Send unit back for repair! 

6.2. During operation

6.2.1. Data error

7.1.1. Technical error; Measured value 1 underflow

The error message can have different origin.

Date of error	02.11.07
Time of error	16:11:10
Measuring circuit 1 or 2	 Data error
Error description	Meas. value 1 Underflow

1. press **ok** button more than 2 seconds, the error is confirmed and the display changes back to last active menu point

The mA output falls to the value programmed under menu point 8.3!

Description of 1 st meas. circuit position	1 Pos. QLA12345679
Description of 1 st meas. value	Analog output 1
Non display of meas. value	---.- % Lo ↓
Error display	Menu ▼▲▼
ok button-functions / active keys	Press Ok to change to menu

Limit value low alarm is reached
Arrow down ↓ **signals** : Meas. range underflow

use the ▲▼ buttons to scroll within display mode

Description of the outputs	Analog outputs
Description of 1. and 2. meas. value	1 00.50 mA
Display of actual value of current outputs	2 11.20 mA
ok button-functions / active keys	Menu ▲▼
	Press Ok to change to menu

use the ▲▼ buttons to scroll within display mode



LEDs on measuring electronic MTI are dark/OFF

1. Short circuit or circuit break. Change connection wires on clamp 1 / 2 of probe electronic.

⌋ **Check connections of measuring electronic MTI**

2. Hazardous area output microprocessor unit **mipromex** or measuring electronic MTI defective

⇒ **Send unit back for repair!** 

The electronic insert MTI is plugged in the blue protection housing. Loosen the two outer M4-screws and remove the electronic insert MTI laterally towards the cable gland.



LED's on measuring electronic MTI are ON

3. Range monitoring did respond, measured value <10

⌋ **Check with 0-point-function at menu item 5.3. , perform a new zero adjust**

4. Coax cable or probe defective (circuit break)

⇒ **Send coax cable and probe back for repair!** 



Calibration of MTI was possible, microprocessor unit mipromex showing fault or after power cut showing measured value underflow (no measure):

5. Hazardous area data input of **mipromex** defective;


⇒ **Send mipromex unit back for repair!** 

7.1.1.

Technical error; Measured value 1 overflow


The error message can have different origin.

Date of error
Time of error
Measuring circuit 1 or 2
Error description

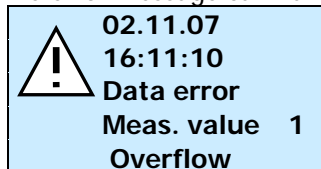



1. press **ok** button more than 2 seconds, the error is confirmed and the display changes back to last active menu point

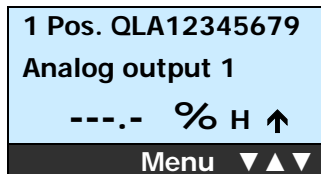Description of 1st meas. circuit position
Description of 1st meas. value
Non display of meas. value
Error display
ok button-functions / active keys




- Limit value high alarm is reached
Arrow up ↑ signalizes : **Meas. range overflow**

Press **Ok** to change to menu



use the   buttons to scroll within display mode

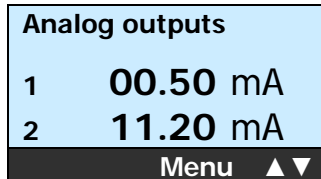Description of the outputs
Description of 1. and 2, meas. value
Display of actual value of current outputs



ok button-functions / active keys

Press **Ok** to change to menu

use the   buttons to scroll within display mode

⌋ **Check probe, product intrusion**

**LEDs on MTI measuring electronic are ON**

6. Range control active, measured value >3750

⇒ **Scheck with 0-point function under Menu 5.3, perform new basic calibration**

⇒ Probe not covered (empty), coax cable or probe defective (coax plug wet)

⇒ Fault occurs only when probe covered (full): Impedance in function of product too high:



Send probe back for repair!

6.2.2. Display error**Faulty or no display on the LCD display**

1. Restart the program after 5 seconds of mains interruption.

6.2.3. Radio equipment


Radio/wireless equipment should not be operated in the immediate vicinity of the microprocessor unit **mipromex**, of an open MTI measuring electronic or of the bar probe (measurements can be affected)



Minimum distance 1 to 2 m

7. Wiring diagram

7.1. Measuring electronic/probe with fix connection

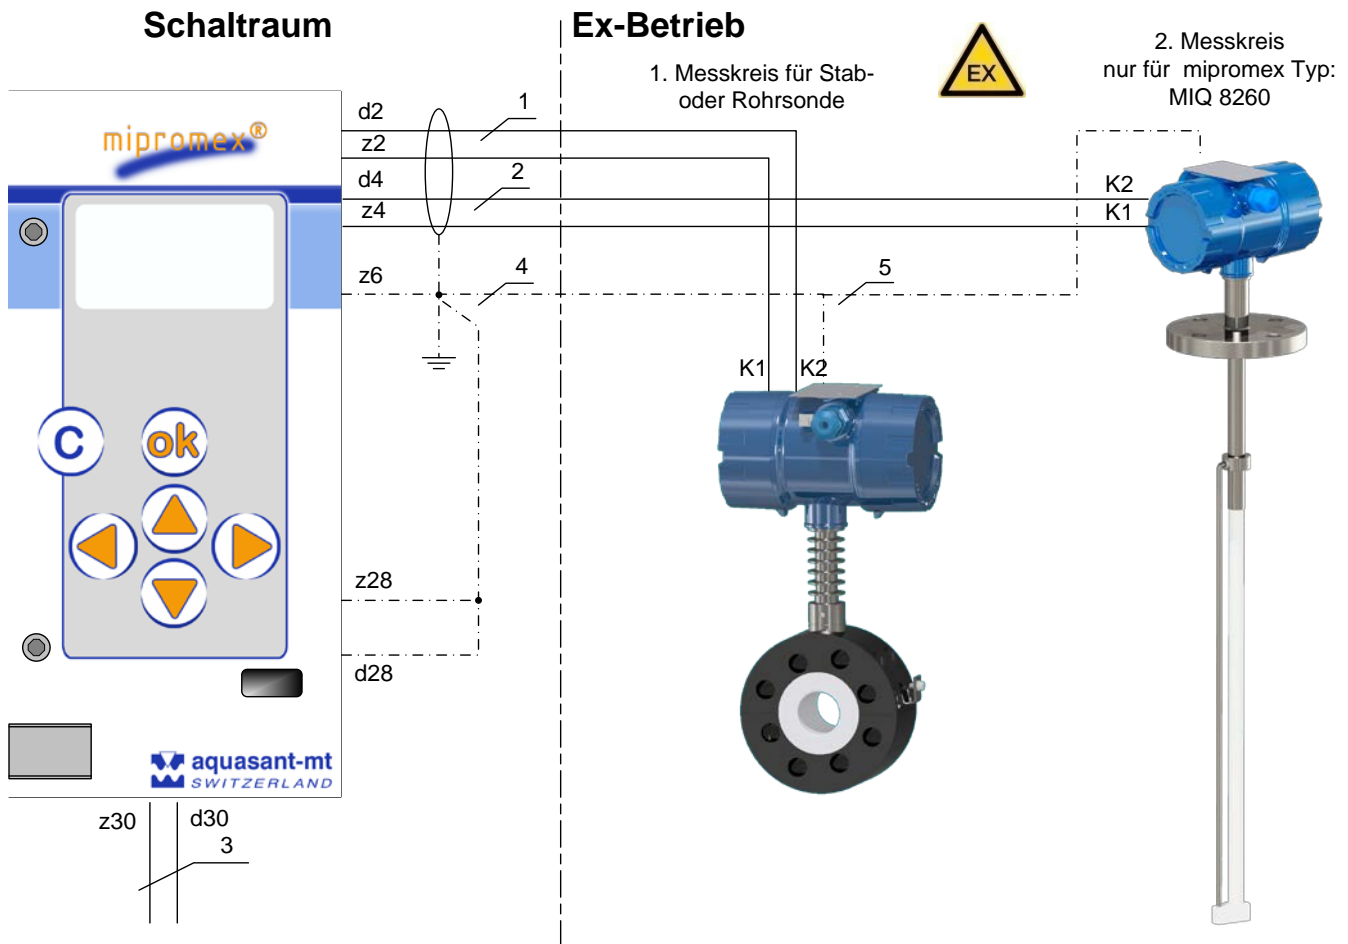


Pic. 4 Wiring diagram

1. 2 x 0.75 mm² shielded (both sides earthed in switch room and probe head)
2. MTI housing and probe are connected to the (factory/plant) equipment earths
3. Mains 24 V AC 50/60 Hz /DC ±10 % control voltage, polarity independent, without inductive load
4. Equipotential bond
An equipotential bond must be fitted between the control room earth and the equipment earth (condition of hazardous area protection and for accurate data transmission)

7.2. Connections to female multipoint connector with 32 poles, type: MAT 419*

Microprocessor units with one measuring circuit input
Connections to female multipoint connector FI 32

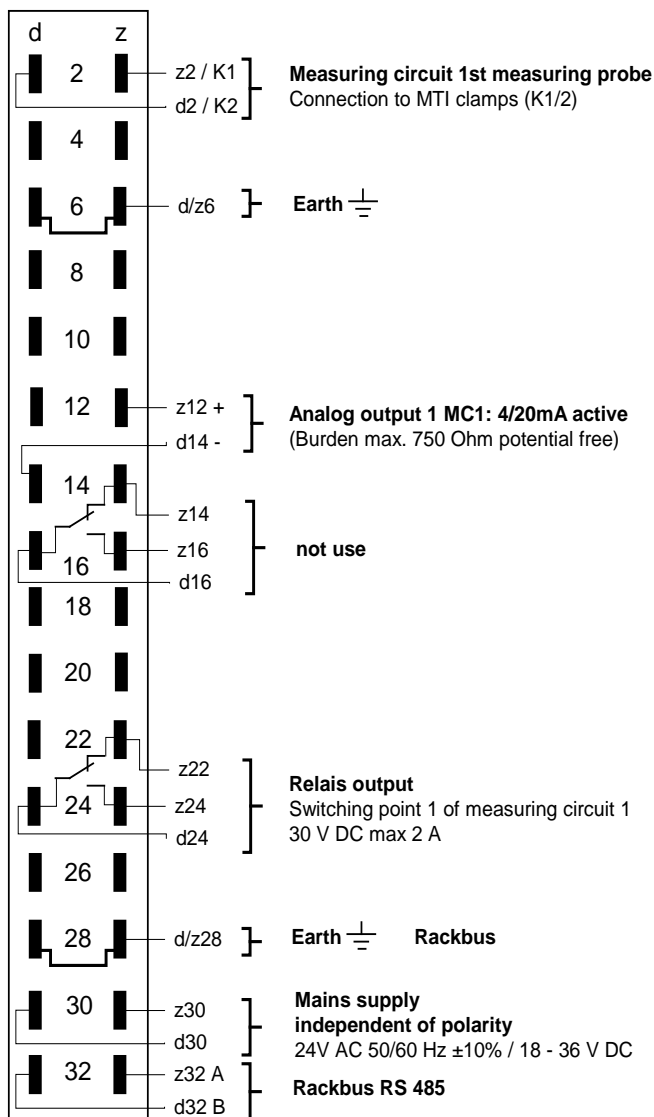

ELECTRICAL DATA

Euro plug-in card pin assignment

24 V-Version

Error message programmable in
 0.1 mA-steps;
 0.5 – 3.9 / 20.1 – 22 mA

Pic. 5 FI 32 female multipoint connector to MAT 4190

Switch point 1 for measuring circuit 1 **FSL** (Fail Safe Low) **Lo-Alarm**
 Switch point 1 for measuring circuit 1 **FSH** (Fail Safe Low) **Hi-Alarm**
 Relay 1 disabled (measured value < limit switch value)

Switch point 2 not activated

Technical error level of analog output according to parameterization

Relay 1/2 disabled

7.3. Printed circuit board for 19"-Rack, Monorack, Wall- and Table Top housing

The Cage Clamp® connection clamps for cable diameter 0.08 – 2.5 mm² bared length 5 – 6 mm /0.22 in (without cable cover) are mounted with a special pre spanning tool.


Color coding:

- To the **blue** clamps: connection of the intrinsically safe field circuit. This one being allowed, with connection lines in accordance to DIN EN 60079-14, to be routed into the hazardous area.
- The **black/orange**- clamps are polarity independent current- inputs or -outputs

Dimension: H x B x T 137 x 77 x 210 mm / for 19"-plug in module Euro 3 HE/12TE profundity 160 mm

Anschluss an: Microprocessor unit mipromex


Artikel-Nr.: 02.03.18.011

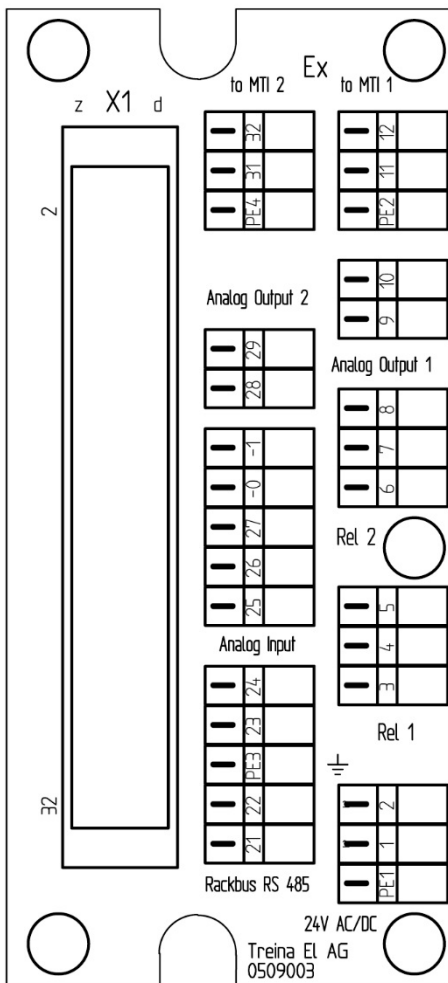

- | Relay | Opto-e. coupler | |
|---|-----------------|------------|
| 1. Mains 24 V AC/DC 50/60 Hz (polarity independent) | | FI32: d/z6 |
| 2. Mains 24 V AC/DC 50/60 Hz (polarity independent) | | FI32: z30 |
| 3. 1 NO | output E- | FI32: z24 |
| 4. 1 COM | output C+ | FI32: d24 |
| 5. 1 NC | - | FI32: z22 |
| 6. 2 NO | output E- | FI32: z16 |
| 7. 2 COM | output C+ | FI32: d16 |
| 8. 2 NC | - | FI32: z14 |
| 9. MC1 analog output 1 - | | FI32: d14 |
| 10. MC1 analog output 1+ | | FI32: z12 |
| 11. MC1 MTI 1 K1 | | FI32: z2 |
| 12. MC1 MTI 1 K2 | | FI32: d2 |
| 21. | | FI32: z32 |
| 22. | | FI32: d32 |
| 23. Analog input - | | FI32: d18 |
| 24. Analog input + | | FI32: d12 |
| 25. Digital input 1 (+24 V) | | FI32: d10 |
| 26. Digital input 2 (+24 V) | | FI32: z10 |
| 27. Digital input 3 (+24 V) | | FI32: d8 |
| -0 Digital input D1-3 (0 V) | | FI32: z8 |
| -1 Digital input D1-3 (0 V) | | FI32: z8 |
| 28. MC2 Analog output 2 - | | FI32: d22 |
| 29. MC2 Analog output 2+ | | FI32: z20 |
| 31. MC2 MTI 2 K1 | | FI32: z4 |
| 32. MC2 MTI 2 K2 | | FI32: d4 |




Pic. 6 Connection print to mipromex

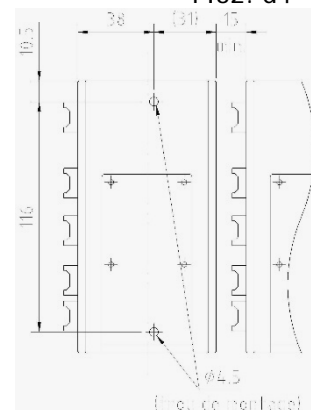

7.4. Earthing of microprocessor units and probes

Equipotential bond and correct earthing for the hazardous area protection and against disturbances of the data transmission

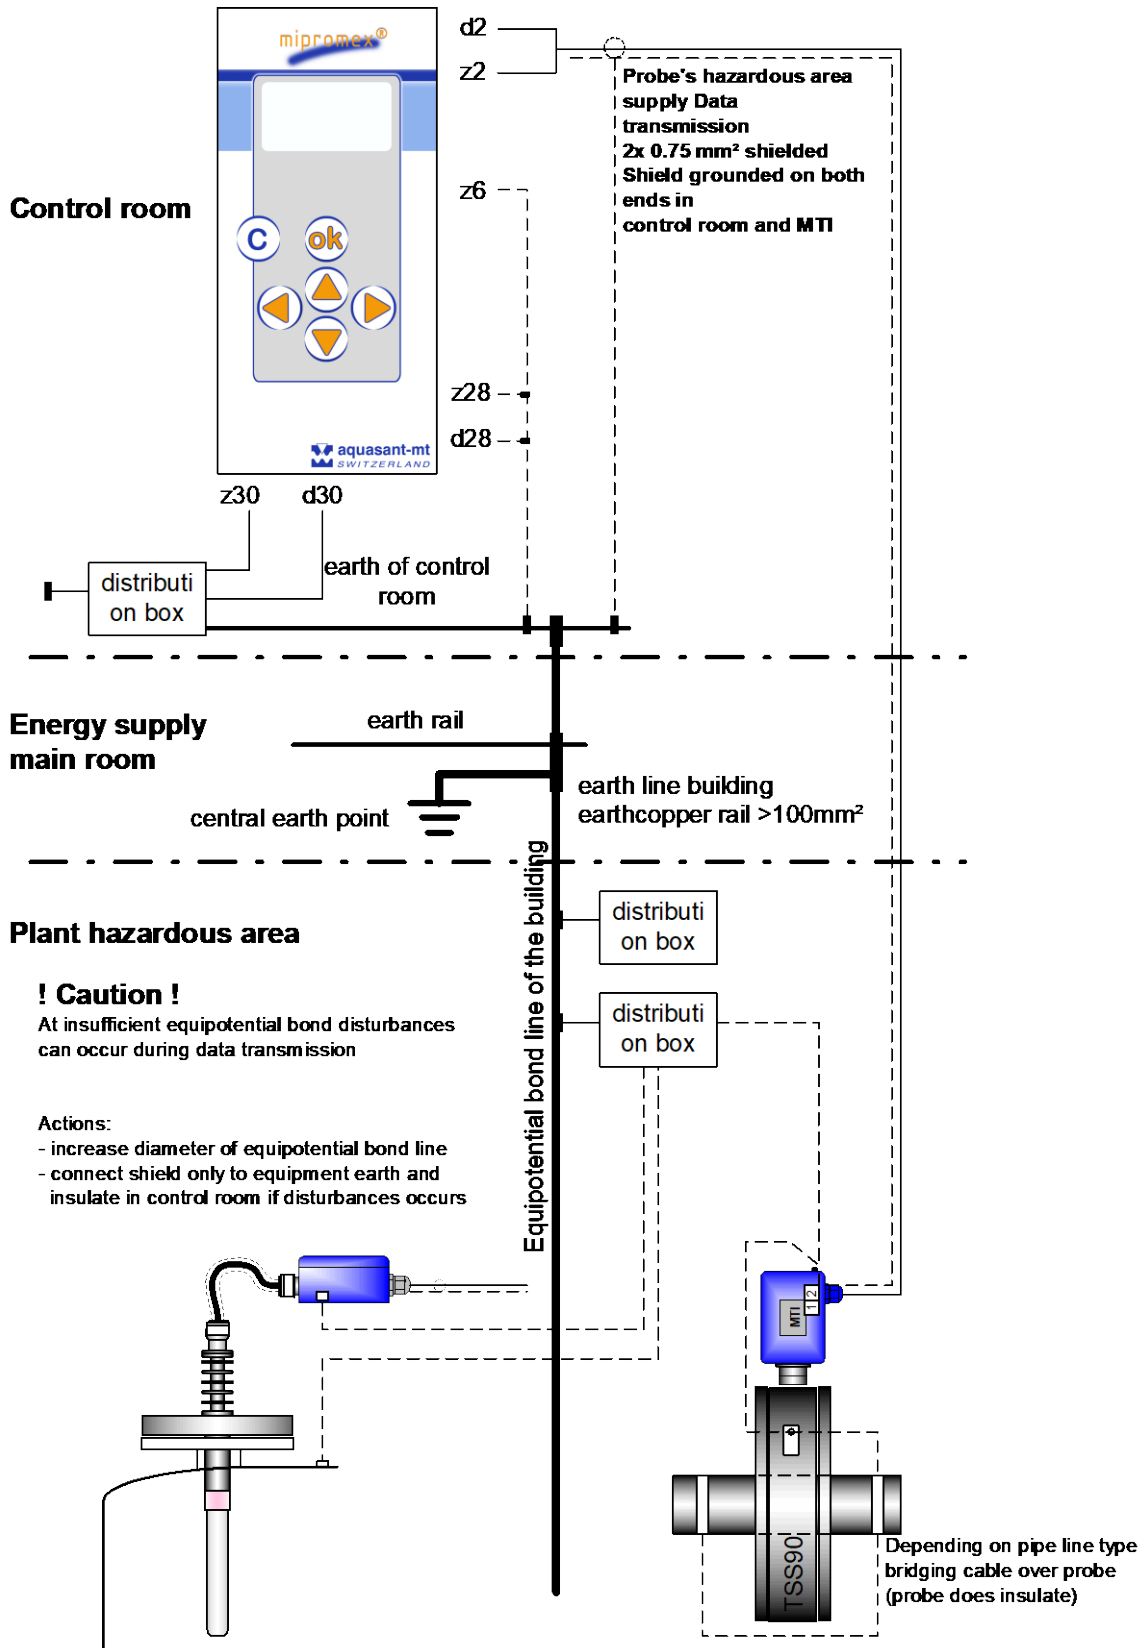

Pic. 7 Earthing principle

8. Technical Data

8.1. mipromex Analog transmitter type: MAT 419x

Construction

19"-plug in module, with aluminum-steel housing; IP 20

Assembly

19"-Rack type MR 7; 3 HE (Europ.sizes)
 Monorack type MRM2; plastic housing for DIN-rail- or wall mounting.
 Front plate fitting with Bopla housing.
 Compact or table top housing

Purpose

- analog transmitter with intrinsically safe supply for one measuring electronic MTI xx. Transformation of a digital measuring signal into an analog signal with measuring range spread
- analog output 4 – 20 mA
- menu driven, multi language unit
- hazardous area (Ex) supply for one measuring electronic MTI xx
- shielded 19" plug in module
- one open collector outputs NPN

Operation/Display

Film keypad-front plate with graphical LCD-display, backlit, 6 buttons for data and parameter input

Data saving during power cuts

Battery buffer max. 10 years. Parameter storage into flash at battery failure

Dimensions

Height 3 HE; Width 12 TE
 Front plate: Height x width 128 x 61 mm
 Plug in module: Height x width x depth 100 x 60 x 160 mm
 7 units can be inserted on a 19"-rack

Weight

690 g

Mains supply

24 VAC 50/60 Hz $\pm 10\%$ / 24 VDC Range 18 – 36 VDC
 independent of polarity

Switch on current

momentary (1ms) approx. 1A

Power input t

ca. 3.4 VA (I = 140 mA)

Fuses

8.5 x 8.5 mm miniature fuse MST 400 mA

Hazardous area supply and signal transmission

[Ex ia] IIC Pulse modulated supply signal
 open circuit voltage max. 18.9 V; typically 17 V
 short circuit current max. 49 mA; typically 40 mA

[Ex d ia], Pulse modulated supply signal
 open circuit voltage max. $U \leq 19.3$ V; typ. 17 V
 short circuit current max. $I \leq 75$ mA; typ. 70 mA

Signal transmission

1 measuring circuit, pulse modulated supply signal

Signal line short circuit

power input max. MAT 4110: 160 mA

Ambient temperature

0 °C ... 45 °C

Storage temperature

-20 °C ... +45 °C, ideally 20 °C

Measurement range

0 – 3700 pulses

Data display

MeV 0 – 3700

Switching hysteresis

1 pulse = 0.028 pF for the 100 pF measuring range

Connection

32 pole FI connector, coding facility

Relaysoutput

1 relay per measuring point with a changeover contact for the limit value. Example: min./max. Deviation min. or max. selectable safety value. Switching voltage 30 Vdc /2 A, I/O=2kV, -40 to 85°C

Analog output

one active 4 – 20 mA output, max.working resistance/burden 750 Ω , not for hazardous area, with potential separation, tech. fault 0.5 – 4 / 20 - 22 mA adjustable

Interface

RS 232 / RS 485

Monitoring

Self-monitoring detection system for: defective probe; short circuit/interruption signal supply to hazardous area (cable break security); measurement range; main power interruption
mipromex -error messages

Index**I**

1 measuring circuit 14

2

2 measuring circuits 14
2nd measuring circuit, activation 22

A

Activation code 22
Activation code, Menu- 16
Activation of 2nd measuring circuit 22
Active dataset, protocol, Menu- 17
Active part 11
Ambient temperature 42
Analog output 42
Analog output 1 (display) 14
Analog output 2 (display) 14
Analog outputs %(display) 14
Analog outputs galvanically separated 22
Analog outputs mA (display) 14
Aquasant Measuring Technique Ltd, Switzerland ii
Aquasant Messtechnik AG, Schweiz ii
Aquasant Measure Technique S.A., Suisse ii
aquasant-mt = www.aquasant-mt.com 19
Archive, Menu- 17
Arrow down ↓ signalizes
 Meas. range underflow 35
Arrow up ↑ signalizes
 Meas. range overflow 36
Assembly 42

B

Bar probe 11
Basic equalization 32
Basic settings 19
basic settings, Menu 16
Battery type 23
Battery type, Menu 16
Burden 750 Ohms- 27

C

Calculation parameters, Menu- 17
Cleaning of units 7
Code parameter, Menu- 16, 17, 18
Code, activation 22
Code, type 8, 9, 10, 16
Commissioning 30
Commissioning according to..., Menu 17
Commissioning, with a bar probe 31
Commissioning, with a pipe probe TSS90 30
Conductivity 11
Connection 42

Connection to female multipoint connector 39
Construction 42
Contact- 21
Contact information, Menu- 16
Controller function, Menu- 17

D

Data display 42
Data error- 35
Data error, measuring value overflow 28
Data error, measuring value underflow 28
Data input, structure 13
Data saving during power cuts 42
Detection of oil in process or rain water 30
Detection of water in petrochemical products 30
Device specs 22
Device specs, Menu 16
Device type (display) 14
Device type MAT 22
Diagnosesystem 28
Diagnostic system 35
Dielectrical constant 11
Dimensions 42
Display at switch on 14
Display modes, Menu 18
Display, Analog output 1 14
Display, Analog output 2 14
Display, Analog outputs mA 14
Display, Device type 14
Display, error 37
Display, software release 22
Display, type code 23
Display, Zero point MeV 32
dry and clean (probe must be...) 24, 30, 31, 32
Dynamische Messwertverarbeitung 12

E

Earthing of...- 41
Electronic calibration 32
Equipotential bond 38, 41
equipotential bond line 41
Error level, programmable- 28
Error message mA output, Menu 17
Error, technical- 28
Error, technical- level 39

F

factory settings 21
Factory settings, Menu 16
Fail Safe High 27
Fail Safe Low 27
Fault finding 28, 35
Fault finding, after power on 35
Fault finding, data error 35
Fault finding, operation 35
Foam detection 31
FSL Fail Safe Low 39
FSL/FSH position 27

Function	11
Fuses	42

G

Graphic display	14
-----------------------	----

H

Hardware, types.....	8, 22
Hazardous Area / Plant	38
Hazardous Area protection	6
Hazardous area supply and signal transmission	42
Hi Alarm High Low.....	27

I

Impedance, bar probe	11
Impedance, function.....	11
Impedance, measured value	11
Impedance, pipe probe.....	11
Impedance, probe	6
Impedance, sum signal.....	11
Impedance, too high, fault	37
Information / Notice	3
Initialize unit.....	21
Input / changing of chracters	13
Input field	13
Input Pos. No.....	24
Inspection release of the parameters	33
Installation	6
Interface	42

K

Key -C- =/back/delete/	13
Key description	13
Key -down-	13
Key functions	13
Key in Password, (display)	19
Key -left-	13
Key -OK-	13
Key -right-	13
Key -up-	13
Keypad.....	6
Keypad buttons.....	11
Keypad frontplate.....	42

L

Language, 4 th , to program	13
Language, Menu	16
Language/Sprache	19
Languages Deutsch/English/Français.....	13
Lightning	20
Lightning settings.....	20
Lightning, Menu-	16
Limit value.....	25, 26
Limit values, Menu-	17
Lo Alarm Low.....	27
Load parameter set	21

M

mA output, simulation	27
mA, active current output	27
mA, programmable error level output	28
Mains supply	42
Maintenance.....	7
MAT 4110	22
MAT 4110/220.....	22
MAT 4190, technical data	42
MAT 4220	22
MAT 4240	22
Measured value display-	14
Measured value old probe.....	24
Measurement range	42
Measuring circuits, quantity, Menu	16
Measuring range.....	11, 25
Measuring range, end point	25
Measuring range, Menu.....	17
Measuring range, starting point.....	25
Measuring span-	24
Measuring span acceptance, push button.....	24
Menu Activation code	16
Menu Active dataset, protocol	17
Menu Archive	17
Menu Calculation parameters	17
Menu Code.....	30, 31
Menu Code parameter	16, 17, 18
Menu Controller function	17
Menu description,-	19
Menu Limit values.....	17
Menu parameter settings.....	15
Messwertverarbeitung	12
Monitoring	42
Multipoint connector, 32 poles	39

N

NAMUR EN53	22
Number of measuring circuits	23

O

Oil detection, with a float	31
Oil in Water, detection-	30
OK button (key -OK-)	3, 13, 15
Old probe, measured value.....	24
Operation / Display	42
Opto-electronic coupler	6, 11, 26, 27, 40
Opto-electronic coupler, de-energized.....	27
Opto-electronic coupler, define security settings	27
Opto-electronic coupler, switched on	27

P

Parameter	13
Parameter set, load.....	21
Parameter set, store-	21
Parameter settings, Menu.....	15
Parameter values.....	13
Parameterization.....	13
Password	19
Password, key-in, change	20
Password, modify	20

Password,modify, Menu	16
Passwort input	15
PC software	13
Plant, Hazardous Area	38
Power Input	42
Printed circuit board	40
Probe already soiled with products, (settings)	30, 31
Probe factor	24
Probe type 1 / 2	23
Probes, without reference electrode	32
Product	11
Program messages	3
Program structure with parameters	16
Programmable error level mA output	28
Pulses	11
Purpose	42

R

Rack, 19	30
Rack, Monorack	30
Radio equipment and transmitter-	37
Relaysoutputs	42

S

Safety level switch	12
Second measuring circuit, activation	22
Selec measuring circuit	25
Select language	13
Select measuring circuit	23, 25, 27
Serial No 1 / 2	23
Serial number and system verify, Menu	16
Serial number system verify	22
Service parameter basics,Menu	17
Settings, basic, Menu	16
Settings, if probe already soiled with products	30, 31, 32
Setup	6
Signal filter-	25
Signal line short circuit	42
Signal settings	23
Signal settings, Menu	16
Signal transmission	42
Simulation of mA output	27
Software	8
Software (Display)	22
Software, activation	22
Software, codes	9
Software, dutiable	22
Software, functions	22
Software, marking	22
Software, operating	10
Software, packages	22
Software, PC	13
Software, release (Display)	22
Software, standard	9
Software, versions	10, 16

Soiled and uncleaned probes, settings	32
Statische Messwertverarbeitung	12
Storage temperature	42
Store parameter set	21
Structure Data input-	13
Surface oil, detection	31
Switch on current	42
Switching hysteresis	42
Symbols	3

T

Technical Data	42
Technical error	28
Technical error level	39
Technical error, Measured value 1 overflow	36
Technical error, Measured value 1 underflow	35
Test and certification	42
Test functions	27
Test functions, Menu	17
Text input	13
Time, drop off or on raise delay	26
Time/Date	20
Time/Date, Menu	16
Type code	8, 9, 10, 16
Type code, (Display)	23
Types, of hardware	8, 22

U

<i>Using this manual</i>	3
--------------------------------	---

V

Version, 24 V	39
Version, manual	ii
Version, software	10, 16, 22

W

Warranty claims	7
Waste disposal of...-	7
Water in Oil, detection	30
Weight	42
Wiring diagramm	38

Z

Zero point acceptance, push button	24
Zero point input, manual	24
Zero point MeV (display)	32
Zero point, accept actual	30

List of tables:

Chart 1 Symbol description	3
Chart 2 Key functions	13
Chart 3 Display	13
Chart 4 Program structure	18
Chart 5 Fail Safe settings	27
Chart 6 Commissioning of water detection	30

Chart 7	Commissioning of oil detection	30
Chart 8	Commissioning of oil layer detection	31
Chart 9	Commissioning of foam detection.....	31
Chart 10	Electronic calibration operating sequences	32

List of pictures:

Pic. 1	mipromex	8
Pic. 2	static measure processing mode.....	12
Pic. 3	dynamic processing mode.....	12
Pic. 4	Wiring diagram	38
Pic. 5	FI 32 female multipoint connector to MAT 4190	39
Pic. 6	Connection print to mipromex	40
Pic. 7	Earthing principle.....	41

Notes: